

**FoundationOne[®]CDx
Technical Information**

Foundation Medicine, Inc.
150 Second Street, Cambridge, MA 02141
Phone: 617.418.2200

Intended Use

FoundationOne[®]CDx (F1CDx) is a qualitative next generation sequencing based *in vitro* diagnostic test that uses targeted high throughput hybridization-based capture technology for detection of substitutions, insertion and deletion alterations (indels), and copy number alterations (CNAs) in 324 genes and select gene rearrangements, as well as genomic signatures including microsatellite instability (MSI) and tumor mutational burden (TMB) using DNA isolated from formalin-fixed, paraffin embedded (FFPE) tumor tissue specimens. The test is intended as a companion diagnostic to identify patients who may benefit from treatment with the targeted therapies listed in Table 1 in accordance with the approved therapeutic product labeling. Additionally, F1CDx is intended to provide tumor mutation profiling to be used by qualified health care professionals in accordance with professional guidelines in oncology for patients with solid malignant neoplasms. Genomic findings other than those listed in Table 1 are not prescriptive or conclusive for labeled use of any specific therapeutic product.

Table 1. Companion diagnostic indications

Tumor Type	Biomarker(s) Detected	Therapy
Non-small cell lung cancer (NSCLC)	<i>EGFR</i> exon 19 deletions and <i>EGFR</i> exon 21 L858R alterations	Gilotrif [®] (afatinib), Iressa [®] (gefitinib), Tagrisso [®] (osimertinib), or Tarceva [®] (erlotinib)
	<i>EGFR</i> exon 20 T790M alterations	Tagrisso [®] (osimertinib)
	<i>ALK</i> rearrangements	Alecensa [®] (alectinib), Xalkori [®] (crizotinib), or Zykadia [®] (ceritinib)
	<i>BRAF</i> V600E	Tafinlar [®] (dabrafenib) in combination with Mekinist [®] (trametinib)
	<i>MET</i> single nucleotide variants (SNVs) and indels that lead to <i>MET</i> exon 14 skipping	Tabrecta [™] (capmatinib)
Melanoma	<i>BRAF</i> V600E	Tafinlar [®] (dabrafenib) or Zelboraf [®] (vemurafenib)
	<i>BRAF</i> V600E and V600K	Mekinist [®] (trametinib) or Cotellic [®] (cobimetinib) in combination with Zelboraf [®] (vemurafenib)
Breast cancer	<i>ERBB2</i> (HER2) amplification	Herceptin [®] (trastuzumab), Kadcyla [®] (ado-trastuzumab-emtansine), or Perjeta [®] (pertuzumab)

	<i>PIK3CA</i> C420R, E542K, E545A, E545D [1635G>T only], E545G, E545K, Q546E, Q546R, H1047L, H1047R, and H1047Y alterations	Piqray [®] (alpelisib)
Colorectal cancer	<i>KRAS</i> wild-type (absence of mutations in codons 12 and 13)	Erbix [®] (cetuximab)
	<i>KRAS</i> wild-type (absence of mutations in exons 2, 3, and 4) and <i>NRAS</i> wild type (absence of mutations in exons 2, 3, and 4)	Vectibix [®] (panitumumab)
Ovarian cancer	<i>BRCA1/2</i> alterations	Lynparza [®] (olaparib) or Rubraca [®] (rucaparib)
Cholangiocarcinoma	<i>FGFR2</i> fusions and select rearrangements	Pemazyre [™] (pemigatinib)
Prostate cancer	Homologous Recombination Repair (HRR) gene (<i>BRCA1</i> , <i>BRCA2</i> , <i>ATM</i> , <i>BARD1</i> , <i>BRIP1</i> , <i>CDK12</i> , <i>CHEK1</i> , <i>CHEK2</i> , <i>FANCL</i> , <i>PALB2</i> , <i>RAD51B</i> , <i>RAD51C</i> , <i>RAD51D</i> and <i>RAD54L</i>) alterations	Lynparza [®] (olaparib)
Solid tumors	TMB \geq 10 mutations per megabase	Keytruda [®] (pembrolizumab)
	<i>NTRK1/2/3</i> fusions	Vitrakvi [®] (larotrectinib)

The test is also used for detection of genomic loss of heterozygosity (LOH) from formalin-fixed, paraffin-embedded (FFPE) ovarian tumor tissue. Positive homologous recombination deficiency (HRD) status (F1CDx HRD defined as tBRCA-positive and/or LOH high) in ovarian cancer patients is associated with improved progression-free survival (PFS) from Rubraca (rucaparib) maintenance therapy in accordance with the Rubraca product label.

The F1CDx assay is performed at Foundation Medicine, Inc. sites located in Cambridge, MA and Morrisville, NC.

Contraindication

There are no known contraindications.

Warnings and Precautions

- Alterations reported may include somatic (not inherited) or germline (inherited) alterations; however, the test does not distinguish between germline and somatic alterations. The test does not provide information about susceptibility.
- Biopsy may pose a risk to the patient when archival tissue is not available for use with the assay. The patient's physician should determine whether the patient is a candidate for biopsy.
- Reflex testing to an alternative FDA approved companion diagnostic should be performed for patients who have an *ERBB2* amplification result detected with copy number equal to 4 (baseline ploidy of tumor +2) for confirmatory testing. While this result is considered negative by FoundationOne[®]CDx (F1CDx), in a clinical concordance study with an FDA approved FISH test, 70% (7 out of 10 samples) were positive, and 30% (3 out of 10 samples) were negative by the FISH test with an average ratio of 2.3. The frequency of *ERBB2* copy number 4 in breast cancer is estimated to be approximately 2%¹.

¹Multiple references listed in <https://www.mycancergenome.org/content/disease/breast-cancer/ERBB2/238/>) report the frequency of HER2 overexpression as 20% in breast cancer. Based on

the F1CDx HER2 CDx concordance study, approximately 10% of HER2 amplified samples had copy number 4. Thus, total frequency is conservatively estimated to be approximately 2%.

Limitations

- For *in vitro* diagnostic use.
- For prescription use only. This test must be ordered by a qualified medical professional in accordance with clinical laboratory regulations.
- A negative result does not rule out the presence of a mutation below the limits of detection of the assay.
- Samples with <25% tumor may have decreased sensitivity for the detection of CNAs including *ERBB2*.
- Clinical performance of Tagrisso[®] (osimertinib) in patients with an *EGFR* exon 20 T790M mutation detected with an allele fraction <5% is ongoing and has not been established.
- Concordance with other validated methods for CNA (with the exception of *ERBB2* amplifications and *BRCA1/2* homozygous deletions) and gene rearrangement (with the exception of *ALK*) detection has not been demonstrated and will be provided in the post-market setting. Confirmatory testing using a clinically validated assay should be performed for all CNAs and rearrangements not associated with CDx claims noted in Table 1 of the Intended Use, but used for clinical decision making.
- The MSI-H/MSS designation by FMI FoundationOne[®]CDx (F1CDx) test is based on genome wide analysis of 95 microsatellite loci and not based on the 5 or 7 MSI loci described in current clinical practice guidelines. Refer https://www.accessdata.fda.gov/cdrh_docs/pdf17/P170019B.pdf for additional details on methodology. The threshold for MSI-H/MSS was determined by analytical concordance to comparator assays (IHC and PCR) using uterine, cecum and colorectal cancer FFPE tissue. Patients with microsatellite status of “Cannot Be Determined” should be retested with an orthogonal (alternative) method. The clinical validity of the qualitative MSI designation has not been established.
- TMB by F1CDx is determined by counting all synonymous and non-synonymous variants present at 5% allele frequency or greater (after filtering) and the total number is reported as mutations per megabase (mut/Mb) unit. Observed TMB is dependent on characteristics of the specific tumor focus tested for a patient (e.g., primary vs. metastatic, tumor content) and the testing platform used for the detection; therefore, observed TMB results may vary between different specimens for the same patient and between detection methodologies employed on the same sample. The TMB calculation may differ from TMB calculations used by other assays depending on variables such as the amount of genome interrogated, percentage of tumor, assay limit of detection (LoD), filtering of alterations included in the score, and the read depth and other bioinformatic test specifications. Refer to the SSED for a detailed description of these variables in FMI’s TMB calculation https://www.accessdata.fda.gov/cdrh_docs/pdf17/P170019B.pdf. The clinical validity of TMB defined by this panel has been established for TMB as a qualitative output for a cut-off of 10 mutations per megabase but has not been established for TMB as a quantitative score.
- Decisions on patient care and treatment must be based on the independent medical judgment of the treating physician, taking into consideration all applicable information concerning the patient’s condition, such as patient and family history, physical examinations, information from other diagnostic tests, and patient preferences, in accordance with the standard of care in a given community.
- The test is intended to be performed on specific serial number-controlled instruments by Foundation Medicine, Inc.
- Alterations in polyT homopolymer runs may not be reliably detected in *BRCA1/2*.
- Certain large rearrangements in *BRCA1/2* including large scale genomic deletions (affecting at least one whole exon), insertions or other deleterious genomic rearrangements including inversions or transversion events, may not be detected in an estimated 5% of ovarian cancer patients with *BRCA1/2* mutations by F1CDx.
- Certain potentially deleterious missense or small in-frame deletions in *BRCA1/2* may not be reported under the “CDx associated findings” but may be reported in the “Other alterations and biomarkers identified” section in the patient report.
- Alterations at allele frequencies below the established limit of detection may not be detected consistently.
- Detection of LOH has been verified only for ovarian cancer patients

- Performance of the LOH classification has not been established for samples below 35% tumor content and with LOH scores near the cut-off of 16.
- There may be potential interference of ethanol with LOH detection. The interfering effects of xylene, hemoglobin, and triglycerides on the LOH score have not been demonstrated.
- While the overall positive percent agreement between trial enrollment assays and F1CDx was 84% (37/44), thirty percent (30%) (6/20) of patients enrolled in the VITRAKVI clinical studies using RNA-based NGS detection were negative for *NTRK* fusions by F1CDx. Four of the six patients (4/6 or 60%) that were negative for *NTRK* fusions by F1CDx had a response to larotrectinib. Therefore, F1CDx may miss a subset of patients with solid tumors with *NTRK1/2/3* fusions who may derive benefit from VITRAKVI.
- *NTRK2* fusions per the F1CDx CDx biomarker rules for *NTRK1/2/3* fusions were not well-represented in analytical validation studies.

Test Principle

FoundationOne[®]CDx (F1CDx) is performed exclusively as a laboratory service using DNA extracted from formalin-fixed, paraffin-embedded (FFPE) tumor samples. The assay employs a single DNA extraction method from routine FFPE biopsy or surgical resection specimens; 50-1000 ng of DNA will undergo whole-genome shotgun library construction and hybridization-based capture of all coding exons from 309 cancer-related genes, one promoter region, one non-coding (ncRNA), and select intronic regions from 34 commonly rearranged genes, 21 of which also include the coding exons (refer to Table 2 and Table 3 for the complete list of genes included in F1CDx). In total, the assay detects alterations in a total of 324 genes. Using the Illumina[®] HiSeq 4000 platform, hybrid capture–selected libraries are sequenced to high uniform depth (targeting >500X median coverage with >99% of exons at coverage >100X). Sequence data is then processed using a customized analysis pipeline designed to detect all classes of genomic alterations, including base substitutions, indels, copy number alterations (amplifications and homozygous gene deletions), and select genomic rearrangements (e.g., gene fusions). Additionally, genomic signatures including microsatellite instability (MSI) and tumor mutational burden (TMB), and positive homologous recombination deficiency (HRD) status (tBRCA-positive and/or LOH high) are reported.

Table 2. Genes with full coding exonic regions included in FoundationOne[®]CDx for the detection of substitutions, insertions and deletions (indels), and copy number alterations (CNAs).

<i>ABL1</i>	<i>BRAF</i>	<i>CDKN1A</i>	<i>EPHA3</i>	<i>FGFR4</i>	<i>IKZF1</i>	<i>MCL1</i>	<i>NKX2-1</i>	<i>PMS2</i>	<i>RNF43</i>	<i>TET2</i>
<i>ACVR1B</i>	<i>BRCA1</i>	<i>CDKN1B</i>	<i>EPHB1</i>	<i>FH</i>	<i>INPP4B</i>	<i>MDM2</i>	<i>NOTCH1</i>	<i>POLD1</i>	<i>ROS1</i>	<i>TGFBR2</i>
<i>AKT1</i>	<i>BRCA2</i>	<i>CDKN2A</i>	<i>EPHB4</i>	<i>FLCN</i>	<i>IRF2</i>	<i>MDM4</i>	<i>NOTCH2</i>	<i>POLE</i>	<i>RPTOR</i>	<i>TIPARP</i>
<i>AKT2</i>	<i>BRD4</i>	<i>CDKN2B</i>	<i>ERBB2</i>	<i>FLT1</i>	<i>IRF4</i>	<i>MED12</i>	<i>NOTCH3</i>	<i>PPARG</i>	<i>SDHA</i>	<i>TNFAIP3</i>
<i>AKT3</i>	<i>BRIP1</i>	<i>CDKN2C</i>	<i>ERBB3</i>	<i>FLT3</i>	<i>IRS2</i>	<i>MEF2B</i>	<i>NPM1</i>	<i>PPP2R1A</i>	<i>SDHB</i>	<i>TNFRSF14</i>
<i>ALK</i>	<i>BTG1</i>	<i>CEBPA</i>	<i>ERBB4</i>	<i>FOXL2</i>	<i>JAK1</i>	<i>MEN1</i>	<i>NRAS</i>	<i>PPP2R2A</i>	<i>SDHC</i>	<i>TP53</i>
<i>ALOX12B</i>	<i>BTG2</i>	<i>CHEK1</i>	<i>ERCC4</i>	<i>FUBP1</i>	<i>JAK2</i>	<i>MERTK</i>	<i>NT5C2</i>	<i>PRDM1</i>	<i>SDHD</i>	<i>TSC1</i>
<i>AMER1</i>	<i>BTK</i>	<i>CHEK2</i>	<i>ERG</i>	<i>GABRA6</i>	<i>JAK3</i>	<i>MET</i>	<i>NTRK1</i>	<i>PRKAR1A</i>	<i>SETD2</i>	<i>TSC2</i>
<i>APC</i>	<i>C11orf30</i>	<i>CIC</i>	<i>ERRF1</i>	<i>GATA3</i>	<i>JUN</i>	<i>MITF</i>	<i>NTRK2</i>	<i>PRKCI</i>	<i>SF3B1</i>	<i>TYRO3</i>
<i>AR</i>	<i>CALR</i>	<i>CREBBP</i>	<i>ESR1</i>	<i>GATA4</i>	<i>KDM5A</i>	<i>MKNK1</i>	<i>NTRK3</i>	<i>PTCH1</i>	<i>SGK1</i>	<i>U2AF1</i>
<i>ARAF</i>	<i>CARD11</i>	<i>CRKL</i>	<i>EZH2</i>	<i>GATA6</i>	<i>KDM5C</i>	<i>MLH1</i>	<i>P2RY8</i>	<i>PTEN</i>	<i>SMAD2</i>	<i>VEGFA</i>
<i>ARFRP1</i>	<i>CASP8</i>	<i>CSF1R</i>	<i>FAM46C</i>	<i>GID4 (C17orf39)</i>	<i>KDM6A</i>	<i>MPL</i>	<i>PALB2</i>	<i>PTPN11</i>	<i>SMAD4</i>	<i>VHL</i>
<i>ARID1A</i>	<i>CBFB</i>	<i>CSF3R</i>	<i>FANCA</i>	<i>GNA11</i>	<i>KDR</i>	<i>MRE11A</i>	<i>PARK2</i>	<i>PTPRO</i>	<i>SMARCA4</i>	<i>WHSC1</i>
<i>ASXL1</i>	<i>CBL</i>	<i>CTCF</i>	<i>FANCC</i>	<i>GNA13</i>	<i>KEAP1</i>	<i>MSH2</i>	<i>PARP1</i>	<i>QKI</i>	<i>SMARCB1</i>	<i>WHSC1L1</i>

ATM	CCND1	CTNNA1	FANCG	GNAQ	KEL	MSH3	PARP2	RAC1	SMO	WT1
ATR	CCND2	CTNNB1	FANCL	GNAS	KIT	MSH6	PARP3	RAD21	SNCAIP	XPO1
ATRX	CCND3	CUL3	FAS	GRM3	KLHL6	MST1R	PAX5	RAD51	SOCS1	XRCC2
AURKA	CCNE1	CUL4A	FBXW7	GSK3B	KMT2A (MLL)	MTAP	PBRM1	RAD51B	SOX2	ZNF217
AURKB	CD22	CXCR4	FGF10	H3F3A	KMT2D (MLL2)	MTOR	PDCD1	RAD51C	SOX9	ZNF703
AXIN1	CD274	CYP17A1	FGF12	HDAC1	KRAS	MUTYH	PDCD1LG2	RAD51D	SPEN	
AXL	CD70	DAXX	FGF14	HGF	LTK	MYC	PDGFRA	RAD52	SPOP	
BAP1	CD79A	DDR1	FGF19	HNF1A	LYN	MYCL	PDGFRB	RAD54L	SRC	
BARD1	CD79B	DDR2	FGF23	HRAS	MAF	MYCN	PDK1	RAF1	STAG2	
BCL2	CDC73	DIS3	FGF3	HSD3B1	MAP2K1	MYD88	PIK3C2B	RARA	STAT3	
BCL2L1	CDH1	DNMT3A	FGF4	ID3	MAP2K2	NBN	PIK3C2G	RB1	STK11	
BCL2L2	CDK12	DOT1L	FGF6	IDH1	MAP2K4	NF1	PIK3CA	RBM10	SUFU	
BCL6	CDK4	EED	FGFR1	IDH2	MAP3K1	NF2	PIK3CB	REL	SYK	
BCOR	CDK6	EGFR	FGFR2	IGF1R	MAP3K13	NFE2L2	PIK3R1	RET	TBX3	
BCORL1	CDK8	EP300	FGFR3	IKBKE	MAPK1	NFKBIA	PIM1	RICTOR	TEK	

Table 3. Genes with select intronic regions for the detection of gene rearrangements, one with 3'UTR, one gene with a promoter region and one ncRNA gene.

ALK introns 18, 19	BRCA1 introns 2, 7, 8, 12, 16, 19, 20	ETV4 intron 8	EZR introns 9- 11	KIT intron 16	MYC intron 1	NUTM1 intron 1	RET introns 7-11	SLC34A2 intron 4
BCL2 3'UTR	BRCA2 intron 2	ETV5 introns 6, 7	FGFR1 intron 1, 5, 17	KMT2A (MLL) introns 6-11	NOTCH2 intron 26	PDGFRA introns 7, 9, 11	ROS1 introns 31-35	TERC ncRNA
BCR introns 8, 13, 14	CD74 introns 6- 8	ETV6 introns 5, 6*	FGFR2 intron 1, 17	MSH2 intron 5	NTRK1 introns 8-11	RAF1 introns 4-8	RSPO2 intron 1	TERT Promoter
BRAF introns 7- 10	EGFR introns 7, 15, 24-27	EWSR1 introns 7-13	FGFR3 intron 17	MYB intron 14	NTRK2 Intron 12	RARA intron 2	SDC4 intron 2	TMPRSS2 introns 1- 3

*ETV6 is a common rearrangement partner for NTRK3

Summary and Explanation

FoundationOne[®]CDx (F1CDx) is a broad companion diagnostic (CDx) test for six tumor indications. In addition to use as a companion diagnostic, F1CDx provides cancer relevant alterations that may inform patient management in accordance with professional guidelines. Information generated by this test is an aid in the identification of patients who are most likely to benefit from associated therapeutic products as noted in Table 1 of the Intended Use.

The F1CDx platform employs whole-genome shotgun library construction and hybridization-based capture of DNA extracted from FFPE tumor tissue prior to uniform and deep sequencing on the Illumina[®] HiSeq 4000. Following sequencing, custom software is used to determine genomic variants including substitutions, insertion and deletion variants (indels), copy number alterations (CNAs), genomic rearrangements, microsatellite instability (MSI), tumor mutational burden (TMB), and positive homologous recombination deficiency (HRD) status. The output of the test includes:

Category 1: Companion Diagnostic (CDx) Claims noted in Table 1 of the Intended Use

Category 2: Cancer Mutations with Evidence of Clinical Significance

Category 3: Cancer Mutations with Potential Clinical Significance

Test Kit Contents

The FoundationOne®CDx (F1CDx) test includes a sample shipping kit, which is sent to ordering laboratories. The shipping kit contains the following components:

- Specimen Preparation Instructions and Shipping Instructions
- Return Shipping Label

All other reagents, materials and equipment needed to perform the assay are used exclusively in the Foundation Medicine laboratories. The F1CDx assay is intended to be performed with serial number-controlled instruments.

Sample Collection and Test Ordering

To order FoundationOne®CDx (F1CDx), the Test Requisition Form (TRF) included in the test kit must be fully completed and signed by the ordering physician or other authorized medical professional. Please refer to Specimen Preparation Instructions and Shipping Instructions included in the test kit.

For more detailed information, including Performance Characteristics, please find the FDA Summary of Safety and Effectiveness Data at: https://www.accessdata.fda.gov/cdrh_docs/pdf17/P170019B.pdf

1. Instruments

The F1CDx device is intended to be performed with the following instruments, as identified by specific serial numbers:

- Agilent Technologies Benchbot Workstation with Integrated Bravo Automated Liquid Handler or Hamilton Microlab STAR/STARlet Liquid Handling Workstation
- Beckman Biomek NX^P Span-8 Liquid Handler or Hamilton Microlab STAR/STARlet Liquid Handling Workstation
- Covaris LE220-plus Focused ultrasonicator
- Thermo Fisher Scientific KingFisher™ Flex with 96 Deep-well Head
- Illumina® cBot System
- Illumina® HiSeq 4000 System

2. Performance Characteristics

Performance characteristics were established using DNA derived from a wide range of FFPE tissue types; tissue types associated with CDx indications were included in each study. Table 4 below provides a summary of tissue types included in each study. Each study also included a broad range of representative alteration types for each class of alteration (substitution, insertion and deletion, copy number alterations, and rearrangements) in various genomic contexts across a broad selection of genes as well as analysis of genomic signatures including MSI and TMB. Table 5 provides a summary of genes and alteration types associated with the validation studies.

Table 4. Summary of tissue types included in validation studies.

Tissue or Tumor Type	Limit of Detection	Precision	Pan-Tumor Analysis	NGS Concordance	Inter-Laboratory Concordance	CDx Concordance	DNA Extraction	DNA Stability (part 1)	FFPE Slide Stability	Interfering Substances	Guard Banding/Robustness	Molecular Index Barcodes	Variant Curation	Reagent Stability
Abdomen or Abdominal wall														
Adrenal Gland														
Anus														
Appendix														
Bladder														
Bone														
Brain														
Breast														
Cervix														
Chest wall														
Cholangiocarcinoma										**				
Colon														
Diaphragm														
Duodenum			*											
Ear			*											
Endometrium			*											
Esophagus														
Fallopian Tube														
Gallbladder														
Gastro-esophageal junction														
Head and Neck														
Kidney														
Larynx			*											
Liver														
Lung														
Lymph Node														
Malignant effusions														
Mediastinum														
Nasal Cavity			*											
Omentum														
Ovarian														
Pancreas														
Pancreatobiliary														

Tissue or Tumor Type	Limit of Detection	Precision	Pan-Tumor Analysis	NGS Concordance	Inter-Laboratory Concordance	CDx Concordance	DNA Extraction	DNA Stability (part 1)	FFPE Slide Stability	Interfering Substances	Guard Banding/Robustness	Molecular Index Barcodes	Variant Curation	Reagent Stability
Parotid Gland			*											
Pelvis														
Penis			*											
Pericardium														
Peritoneum														
Pleura			*											
Prostate														
Rare Tissues*														
Rectum			*											
Salivary Gland														
Skin (Melanoma)														
Small Intestine														
Soft Tissue														
Spleen														
Stomach														
Thyroid														
Tongue			*											
Trachea			*											
Ureter														
Uterus														
Vagina														
Vulva														
Whipple Resection														

*Included as "Rare Tissues" in Pan-Tumor Analysis

** Post-market study pending

Table 5. Summary of genes and alteration types included in validation studies.

Genes	Substitutions	Insertion/Deletions	CNAs	Rearrangements	Precision	LoD	NGS Concordance	Inter-lab Concordance	In Silico Study	DNA Extraction	Guard Band	Interfering Substances
ABL1												
ACVR1B												
AKT1												
AKT2												
AKT3												
ALK*												
ALOX12B												
AMER1 (FAM123B)												
APC												
AR												
ARAF												
ARFRP1												
ARID1A												
ASXL1												
ATM												
ATR												
ATRX												
AURKA												
AURKB												
AXIN1												
AXL												
BAP1												
BARD1												
BCL2												
BCL2L1												
BCL2L2												
BCL6												
BCOR												
BCORL1												
BCR												
BRAF												
BRCA1												
BRCA2												
BRD4												
BRIP1												
BTG1												
BTG2												
BTK												
C11orf30 (EMSY)												
CALR												
CARD11												
CASP8												
CBFB												
CBL												
CCND1												
CCND2												
CCND3												
CCNE1												
CD22												
CD274												

Genes	Substitutions	Insertion/Deletions	CNAs	Rearrangements	Precision	LoD	NGS Concordance	Inter-lab Concordance	In Silico Study	DNA Extraction	Guard Band	Interfering Substances
CD70												
CD74												
CD79A												
CD79B												
CDC73												
CDH1												
CDK12												
CDK4												
CDK6												
CDK8												
CDKN1A												
CDKN1B												
CDKN2A												
CDKN2B												
CDKN2C												
CEBPA												
CHEK1												
CHEK2												
CIC												
CREBBP												
CRKL												
CSF1R												
CSF3R												
CTCF												
CTNNA1												
CTNNB1												
CUL3												
CUL4A												
CXCR4												
CYP17A1												
DAXX												
DDR1												
DDR2												
DIS3												
DNMT3A												
DOT1L												
EED												
EGFR												
EP300												
EPHA3												
EPHB1												
EPHB4												
ERBB2												
ERBB3												
ERBB4												
ERCC4												
ERG												
ERRF1												
ESR1												
ETV4												
ETV5												
ETV6												

Genes	Substitutions	Insertion/Deletions	CNAs	Rearrangements	Precision	LoD	NGS Concordance	Inter-lab Concordance	In Silico Study	DNA Extraction	Guard Band	Interfering Substances
EWSR1												
EZH2												
EZR												
FAM46C												
FANCA												
FANCC												
FANCG												
FANCL												
FAS												
FBXW7												
FGF10												
FGF12												
FGF14												
FGF19												
FGF23												
FGF3												
FGF4												
FGF6												
FGFR1												
FGFR2												
FGFR3												
FGFR4												
FH												
FLCN												
FLT1												
FLT3												
FOXL2												
FUBP1												
GABRA6												
GATA3												
GATA4												
GATA6												
GID4 (C17orf39)												
GNA11												
GNA13												
GNAQ												
GNAS												
GRM3												
GSK3B												
H3F3A												
HDAC1												
HGF												
HNF1A												
HRAS												
HSD3B1												
ID3												
IDH1												
IDH2												
IGF1R												
IKBKE												
IKZF1												

Genes	Substitutions	Insertion/Deletions	CNAs	Rearrangements	Precision	LoD	NGS Concordance	Inter-lab Concordance	In Silico Study	DNA Extraction	Guard Band	Interfering Substances
INPP4B												
IRF2												
IRF4												
IRS2												
JAK1												
JAK2												
JAK3												
JUN												
KDM5A												
KDM5C												
KDM6A												
KDR												
KEAP1												
KEL												
KIT												
KLHL6												
KMT2A (MLL)												
KMT2D (MLL2)												
KRAS												
LTK												
LYN												
MAF												
MAP2K1												
MAP2K2												
MAP2K4												
MAP3K1												
MAP3K13												
MAPK1												
MCL1												
MDM2												
MDM4												
MED12												
MEF2B												
MEN1												
MERTK												
MET												
MITF												
MKNK1												
MLH1												
MPL												
MRE11A												
MSH2												
MSH3												
MSH6												
MST1R												
MTAP												
MTOR												
MUTYH												
MYB												
MYC												
MYCL												
MYCN												

Genes	Substitutions	Insertion/Deletions	CNAs	Rearrangements	Precision	LoD	NGS Concordance	Inter-lab Concordance	In Silico Study	DNA Extraction	Guard Band	Interfering Substances
MYD88												
NBN												
NF1												
NF2												
NFE2L2												
NFKBIA												
NKX2-1												
NOTCH1												
NOTCH2												
NOTCH3												
NPM1												
NRAS												
NT5C2												
NTRK1												
NTRK2												
NTRK3												
NUTM1												
P2RY8												
PALB2												
PARK2												
PARP1												
PARP2												
PARP3												
PAX5												
PBRM1												
PDCD1												
PDCD1LG2												
PDGFRA												
PDGFRB												
PDK1												
PIK3C2B												
PIK3C2G												
PIK3CA												
PIK3CB												
PIK3R1												
PIM1												
PMS2												
POLD1												
POLE												
PPARG												
PPP2R1A												
PPP2R2A												
PRDM1												
PRKAR1A												
PRKCI												
PTCH1												
PTEN												
PTPN11												
PTPRO												
QKI												
RAC1												
RAD21												

Genes	Substitutions	Insertion/Deletions	CNAs	Rearrangements	Precision	LoD	NGS Concordance	Inter-lab Concordance	In Silico Study	DNA Extraction	Guard Band	Interfering Substances
<i>RAD51</i>												
<i>RAD51B</i> (<i>RAD51L1</i>)												
<i>RAD51C</i>												
<i>RAD51D</i> (<i>RAD51L3</i>)												
<i>RAD52</i>												
<i>RAD54L</i>												
<i>RAF1</i>												
<i>RARA</i>												
<i>RB1</i>												
<i>RBM10</i>												
<i>REL</i>												
<i>RET</i>												
<i>RICTOR</i>												
<i>RNF43</i>												
<i>ROS1</i>												
<i>RPTOR</i>												
<i>RSPO2</i>												
<i>SDC4</i>												
<i>SDHA</i>												
<i>SDHB</i>												
<i>SDHC</i>												
<i>SDHD</i>												
<i>SETD2</i>												
<i>SF3B1</i>												
<i>SGK1</i>												
<i>SLC34A2</i>												
<i>SMAD2</i>												
<i>SMAD4</i>												
<i>SMARCA4</i>												
<i>SMARCB1</i>												
<i>SMO</i>												
<i>SNCAIP</i>												
<i>SOCS1</i>												
<i>SOX2</i>												
<i>SOX9</i>												
<i>SPEN</i>												
<i>SPOP</i>												
<i>SRC</i>												
<i>STAG2</i>												
<i>STAT3</i>												
<i>STK11</i>												
<i>SUFU</i>												
<i>SYK</i>												
<i>TBX3</i>												
<i>TEK</i>												
<i>TERC</i>												
<i>TERT promoter</i>												
<i>TET2</i>												
<i>TGFBR2</i>												
<i>TIPARP</i>												

Genes	Substitutions	Insertion/Deletions	CNAs	Rearrangements	Precision	LoD	NGS Concordance	Inter-lab Concordance	In Silico Study	DNA Extraction	Guard Band	Interfering Substances
<i>TMPRSS2</i>												
<i>TNFAIP3</i>												
<i>TNFRSF14</i>												
<i>TP53</i>												
<i>TSC1</i>												
<i>TSC2</i>												
<i>TYRO3</i>												
<i>U2AF1</i>												
<i>VEGFA</i>												
<i>VHL</i>												
<i>WHSC1</i>												
<i>WHSC1L1</i>												
<i>WT1</i>												
<i>XPO1</i>												
<i>XRCC2</i>												
<i>ZNF217</i>												
<i>ZNF703</i>												

2.1 Concordance – Comparison to an Orthogonal Method

The detection of alterations by the FoundationOne[®]CDx (F1CDx) assay was compared to results of an externally validated NGS assay (evNGS). Overall there were 157 overlapping genes between the two assays. The comparison between short alterations, including base substitutions and short indels, detected by F1CDx and the orthogonal method included 188 samples from 46 different tumors. Additional orthogonal concordance data includes:

- 101 breast cancer samples were analyzed to determine concordance specific to *PIK3CA* base substitutions
- 26 cholangiocarcinoma samples were analyzed to determine concordance to an externally validated laboratory developed test specific to *FGFR2* fusions and select rearrangements with additional samples to be completed in the post-market setting
- 168 NSCLC samples were analyzed to determine concordance for detection of qualifying *MET* exon 14 base substitutions and indels
- 120 samples were analyzed to determine concordance specific to HRR alterations (including base substitutions, indels, rearrangements and homozygous deletions)
- 218 samples were analyzed to determine concordance with a CLIA validated whole exome sequencing (WES) assay for detection of TMB \geq 10 mutations per megabase
- 626 solid tumor samples were analyzed to determine concordance of *NTRK1/2/3* fusions. These included 588 samples where F1CDx served as the selection assay (subset 1) and 38 clinical trial samples where local clinical trial assays (LCTAs) served as the selection assay (subset 2).

A summary of Positive Percent Agreement (PPA), Negative Percent Agreement (NPA) and corresponding 95% two-sided exact confidence intervals (CI) is provided in Table 6 below. Differences in variants of unknown significance (VUS) alteration calls between the platforms were noted, and are expected based on differences in filtering employed by F1CDx and evNGS. Negative predictive value and positive predictive value were also calculated and were found to be different than percent agreement because the two platforms filter VUS differently. Discordant alterations not related to VUS filtering were primarily caused by deletions with low allelic fraction in homopolymer regions. The F1CDx variant calling pipeline imposes a filter based on MAF of ≥ 0.10 for indels in homopolymer regions to reduce the likelihood of calling false positives resulting from artifacts introduced by the technology. As such, the difference observed was due to varying filter thresholds between the two platforms. Additional analytical concordance for CDx associated variants is also summarized in Table 6. For *NTRK1/2/3* fusions two analyses were conducted. A primary analysis was focused on the concordance of *NTRK1/2/3* rearrangement detection by F1CDx and evNGS assay where a sample was considered to be positive by F1CDx if any *NTRK1/2/3* rearrangements were present, otherwise it was considered as negative. This analysis was not conducted in accordance with the *NTRK1/2/3* biomarker calling rule but rather to determine the analytical accuracy of *NTRK1/2/3* rearrangement detection as *NTRK1/2/3* fusions are a subset of rearrangements, and the methodology to detect *NTRK1/2/3* rearrangement (fusions and non-fusion rearrangements) is the same. The secondary analysis focused on the concordance of *NTRK1/2/3* rearrangement detection that is predicted to result in an *NTRK1/2/3* fusion event per the F1CDx biomarker rule. In the secondary analysis, a sample was considered F1CDx positive only if it met the *NTRK1/2/3* biomarker rule, otherwise it was considered as F1CDx negative. For additional clinical concordance results for the CDx-associated variants, refer to the Summary of Clinical Studies in Section 3.

Table 6. Concordance summary for short variants inclusive of both substitutions and indels and CDx claims.

	F1CDx+ /evNGS+	F1CDx- /evNGS+	F1CDx+ /evNGS-	F1CDx- /evNGS-	PPA [95% CI]*	NPA [95% CI]*
All short variants	1282	73	375	284218	94.6% [93.3%-95.8%]	99.9% [99.9%-99.9%]
Substitutions	1111	39	334	242540	96.6% [95.4%-97.6%]	99.9% [99.8%-99.9%]
Indels	171	34	41	41678	83.4% [77.6%-88.2%]	99.9% [99.9%-99.9%]
PIK3CA substitutions in Breast Cancer	53	0	0	48	100.00% [93.3%-100.0%]	100.00% [92.6%-100.0%]
FGFR2 fusions**	25	2	1	130	87.08% [61.40%,98.30%]	99.59% [92.87%, 100.00%]
MET exon 14 SNVs and indels	49	0	1	118	100.0% [92.8%-100.0%]	99.2% [95.4%-100.0%]
HRR gene substitutions	35	1	1	8243	97.22% [85.47%, 99.93%]	99.99% [99.93%, 100.00%]
HRR gene indels	75	6	2	17627	92.59% [84.57%, 97.23%]	99.99% [99.96%, 100.00%]
HRR gene rearrangements	10	1	5	1824	90.91% [58.72%, 99.77]	99.73% [99.36%, 99.91%]
HRR gene copy number alterations	20	1	3	1356	95.24% [76.18%, 99.88]	99.78% [99.36%, 99.95%]
NTRK1, NTRK2, NTRK3 fusions	78 ^{#,1}	0 ^{#,1}	18 ^{#,1}	492 ^{#,1}	90.00% [75.00%,100%] ^{#,3}	99.92% [99.92%,99.97%] ^{#,3}
	16 ^{#,2}	2 ^{#,2}	0 ^{#,2}	20 ^{#,2}		

	F1CDx+ /evNGS+	F1CDx- /evNGS+	F1CDx+ /evNGS-	F1CDx- /evNGS-	PPA [95% CI]*	NPA [95% CI]*
	64 ^{##,4}	10 ^{##,4}	4 ^{##,4}	510 ^{##,4}	54.08% [37.94%, 71.37%] ^{##,6}	99.98% [99.96%, 100.00%] ^{##,6}
	15 ^{##,5}	3 ^{##,5}	0 ^{##,5}	20 ^{##,5}		

*The PPA and NPA were calculated without adjusting for the distribution of samples enrolled using the FoundationOne Laboratory Developed Test (F1 LDT), therefore these estimates may be biased upward.

** PPA and NPA were adjusted using a prevalence of 9.6% to account for sampling differential.

#Primary analysis: a sample was considered as positive if an *NTRK1/2/3* rearrangement was detected, otherwise it was considered as negative.

¹Subset 1: samples where F1CDx served as the selection assay. Adjusted PPA and NPA based on an estimated prevalence of 0.32% in the intended use population to account for sampling differences were 100.00% [95%CI: 95.31%, 100.00%] and 99.94% [95%CI: 99.91%, 99.96%] respectively based on the primary analysis.

²Subset 2: clinical trial samples where local clinical trial assays (LCTAs) served as the selection assay. PPA and NPA were 88.89% [95%CI: 67.20%, 96.90%] and 100.00% [95%CI: 83.89%, 100%] respectively based on the primary analysis.

³ The weighted PPA and NPA based on the bootstrapping of the combined dataset 10000 times are shown for the primary analysis.

^{##}Secondary analysis: a sample was considered F1CDx positive only if it met the *NTRK1/2/3* biomarker rule, otherwise it was considered as F1CDx negative.

⁴ Subset 1: samples where F1CDx served as the selection assay. Adjusted PPA and NPA based on an estimated prevalence of 0.32% in the intended use population to account for sampling differences were 13.58% [95%CI: 8.66%, 25.25%] and 99.98% [95%CI: 99.96%, 100.00%] respectively based on the secondary analysis.

⁵ Subset 2: clinical trial samples where local clinical trial assays (LCTAs) served as the selection assay. PPA and NPA were 83.33% [95%CI: 60.78%, 94.16%] and 100.00% [95%CI: 83.89%, 100%] respectively based on the secondary analysis.

⁶ The weighted PPA and NPA based on the bootstrapping of the combined dataset 10000 times are shown for the secondary analysis.

The analysis for concordance of TMB-High (≥ 10 mutations per megabase) detection was performed using a CLIA validated whole exome sequencing (WES) assay. 218 samples were evaluated, of which 89 were not pre-screened by F1CDx (Set A) and 129 were pre-screened by F1CDx (Set B). Concordance results between F1CDx and WES for TMB calling are summarized in Table 7 below.

Table 7. Concordance summary for TMB-High.

	F1CDx+ /evWES+	F1CDx- /evWES+	F1CDx+ /evWES-	F1CDx- /evWES-	PPA [95% CI]	NPA [95% CI]
TMB ≥ 10 mutations per megabase						
Set A	28	7	4	50	80.00% [62.50%,90.62%]	92.59% [82.62%,98.04%]
TMB ≥ 10 mutations per megabase						
Set B¹	23	1	17	88	92.31% [65.74%,100.0%]	90.84% [87.76%,93.99%]

¹PPA and NPA were adjusted using the prevalence of TMB—High estimated at 19%.

The overall PPA and NPA were calculated based on a weighted average of the results (Set A and Set B) in the TMB concordance analysis. Overall PPA was 87.28% (95% CI [64.42%, 96.17%]) and overall NPA was 91.56% (95% CI [85.66%, 95.64%]).

2.2 Concordance – Comparison to FoundationOne[®]

To support the use of retrospective data generated using the FoundationOne[®] (F1 LDT), a concordance study was conducted with FoundationOne[®]CDx (F1CDx). This study evaluated a test set of 165

specimens. PPA and NPA between the F1CDx and F1 LDT, using the F1 LDT assay as the reference method, was calculated for all alterations, as well as for alterations binned by type: short variants, copy number alterations (CNAs) and rearrangements. A total of 2,325 variants, including 2,026 short variants, 266 CNAs and 33 rearrangements were included in the study. The study results are summarized in Table 8 below.

Table 8. Summary of inter-laboratory concordance comparing F1CDx to the F1 LDT.

	F1CDx+/F1 LDT+	F1CDx-/F1 LDT+	F1CDx+/F1 LDT-	F1CDx-/F1 LDT-	PPA	NPA
All variants	2246	33	46	322890	98.6%	99.99%
All short variants	1984	19	23	299099	99.1%	99.99%
Substitutions	1692	10	19	254854	99.4%	99.99%
Indels	292	9	4	44245	97.0%	99.99%
All CNA	230	14	22	19204	94.3%	99.9%
Amplifications	157	10	12	14671	94.0%	99.9%
Losses	73	4	10	4533	94.8%	99.8%
Rearrangements	32	0	1	4587	100.0%	99.98%

The qualitative output for MSI (MSI-H vs. MSS) in the F1 LDT and F1CDx were evaluated. PPA, NPA and Overall Percent Agreement (OPA) of MSI status between the two assays was calculated for all 165 samples. Of the 165 samples, 5 were MSI-H by F1 LDT and 160 were MSS by F1 LDT; there was one discordant sample observed. The discordant sample was called MSS by F1 LDT and MSI-H by F1CDx. After manual review, the discordant case had an MSI score close to the threshold used to classify MSI status. PPA was 100% with a 95% confidence interval (95% CI) of 47.8-100%, NPA was 99.5% with a 95% CI of 96.6%-99.98% and OPA was 99.4% with a 95% CI of 96.7%-99.98%.

2.3 Concordance – LOH and HRD Calling Comparison to FoundationFocus™ CDx BRCA LOH

To support reporting of LOH on FoundationOne® CDx (F1CDx), a concordance study was conducted to compare results of data analyzed using the F1CDx pipeline version 3.1.3 with FoundationFocus™ CDx BRCA LOH (FFocus) data. This analysis included one random replicate from the FFocus LOH sPMA precision samples and one replicate from the FFocus LOH sPMA LoD study for a total of 25 samples. The study results are summarized in Table 9a below.

Table 9a. Summary of LOH calling comparison agreement table.

Agreement	Estimate	95% CI (exact)	Acceptance Criteria
OPA	96.0%	79.6%-99.9%	Low 95%CI >85%
PPA	94.70%	74.0%-99.9%	PPA >90%
NPA	100.00%	54.1%-100.0%	NPA >90%

Concordance for calling HRD status was evaluated by assessing data from the ARIEL3 clinical trial using the F1CDx pipeline. These data are summarized in Tables 9b and 9c below.

Table 9b. Contingency table of F1CDx v3.1.3 HRD status and FFocus HRD status in 518 samples from ARIEL3 study. Numbers in bold are the numbers of cases with determinate HRD outcome by both pipelines, and are used in agreement calculation in Table 9c.

HRD status		F1CDx v3.1.3			
		Indeterminate	Negative	Positive	Sum
FFocus	Indeterminate	22	5	0	27
	Negative	1	156	8	165
	Positive	1	8	317	326
	Sum	24	169	325	518

Table 9c. Agreement between F1CDx v3.1.3 HRD status and FFocus HRD status in 489 samples with determinate HRD outcome by both assays from ARIEL3 study.

	Percent of Agreement [95% CI]
PPA	97.5% [95.2%-98.9%]
NPA	95.1% [90.6%-97.9%]
OPA	96.7% [94.7%-98.1%]

2.4 Tissue Comparability

A large-scale retrospective analysis was conducted, using 80,715 specimens from 43 tissue types, in order to establish the comparability of assay performance across tumor tissue types. The goal of the study was to establish that assay performance after DNA extraction is independent of the tissue type from which the DNA was extracted. The retrospective analysis of data included specimens assayed using the FoundationOne (F1 LDT) assay. DNA extraction, and post-DNA extraction data were assessed for comparability of performance across tissue types. The dataset for analysis consisted of routine clinical samples analyzed using F1 LDT from March 25, 2015 to March 13, 2017.

Thirty-nine of the 43 tissue types had $\geq 90\%$ of specimens passing DNA extraction QC. Specimen DNA extraction pass rates for the remaining four tissue types, lung, pancreas, pelvis and prostate, were 89.6%, 89%, 89%, and 79.7%, respectively. Each of these four tissue types have characteristically small biopsies and may also be more likely to require macro-dissection.

Of specimens entering the assay at Library Construction (LC), 39 of 43 tissue types had $\geq 90\%$ of specimens resulting in a successful patient report being issued. The four tissue types below 90% include pancreatobiliary, appendix, pericardium, and prostate, and had pass rates of 83%, 88%, 79%, and 84%, respectively. For these four tissue types, the most frequent cause of failure was low tumor purity with no alterations detected. The mean LC yields across tissue types were 7,050 ng to 8,643 ng compared to the minimum required 545 ng. The percent of specimens passing the LC QC for each tissue type ranged from 98%-100%. After Hybrid Capture (HC), the mean yields across tissue types ranged from 434 ng to 576 ng, well above the minimum requirement of 140 ng. The percent of specimens passing HC across tissue types ranged from 97%-100%. The average median exon coverage assessed across tissue types ranged from 702X-793X, with percent of specimens passing QC for median coverage across tissue types ranging from 96%-100%. Uniformity of coverage was assessed by calculating the average percent of targets with $>100X$ coverage across tissue types, and ranged from 99.0%-99.8%. The percentage of specimens passing this QC metric ranged from 98%-100%. The average sequencing error rate, assessed across tissue types, is 0.0028-0.0031, well below the required error rate (0.01) for assay acceptance. The pass rate for all tissue types was 100% for error rate. Performance data for this study is summarized in Table 10 below.

Table 10. Summary of post-DNA extraction analysis.

QC Metric Name	F1CDx QC Specification	Mean QC Performance Across Tissue Types	QC Pass Rate Across Tissue Types	Tissue types with ≥90% QC Pass Rate
Overall report Pass/Qualified rate	Pass rate: ≥90% specimens	N/A	79%-98%	39/43 (90.6%)
LC Yield	≥545 ng	7050–8643 ng	98-100%	43/43 (100%)
Library Yield after HC	≥140 ng	434-576 ng	97-100%	43/43 (100%)
Median Exon Coverage	≥250X	702-793X	96-100%	43/43 (100%)
Percent of target >100X coverage	≥95% target at ≥100X coverage	99.0%-99.8% targets	98%-100%	43/43 (100%)
Sequencing error rate	<1%	0.0028-0.0031	100%	43/43 (100%)
Noisy copy number data	N/A*	N/A	93.8-100%	43/43 (100%)

*for information only, not a specification

2.5 Analytical Specificity

2.5.1 Interfering Substances

The robustness of the FoundationOne®CDx (F1CDx) assay process was assessed while evaluating human formalin-fixed paraffin-embedded (FFPE) samples in the presence of exogenous and endogenous interfering substances. Five FFPE specimens representing five tumor types (ovary, lung, colorectal, breast and melanoma) including representative variant types (substitution, indel, amplification, homozygous deletion and rearrangement) were assessed in duplicate (Table 11). An additional 54 short alterations (substitutions and indels) were assessed. The addition of interfering substances including melanin (endogenous), ethanol (exogenous), proteinase K (exogenous), and molecular index barcodes (MIB) (exogenous) was evaluated to determine if they were impactful to F1CDx, and the results were compared to the control (no interferents) condition.

Table 11. Summary of tumor types and variant types included in study.

Tumor Type	Gene (and variant as relevant)	Variant type
CRC	<i>FGFR1</i>	Rearrangement
	<i>BCL2L1</i>	Amplification
	<i>AXIN1</i> c.1058G>A (R353H)	Substitution
	<i>SOX9</i> c.768_769insGG (R257fs*23)	Insertion
Breast cancer	<i>ERBB2</i>	Amplification
	<i>AKT1</i>	Amplification
	<i>CCND1</i>	Amplification
Lung cancer	<i>CDKN2A</i>	Homozygous Deletion
	<i>CDKN2B</i>	Homozygous Deletion
	<i>EGFR</i>	Amplification
Ovarian cancer	<i>BRCA1</i> c.5263_5264insC (Q1756fs*74)	Insertion
	<i>ERCC4</i> c.2395C>T	Substitution
	<i>TP53</i> c.779_779delC (S261fs*84)	Deletion
Melanoma	<i>BRAF</i> c.1799T>A (V600E)	Substitution
	<i>TP53</i> c.856G>A (E286K)	Substitution
	<i>IGF1R</i>	Amplification

Interfering substances included melanin, ethanol, proteinase K, and molecular index barcodes, as noted in Table 12 below. Each of the five FFPE specimens were tested in either two or four replicates each, resulting in a total of 170 data points across the five specimens (10 without interferent, 80 for evaluation of melanin, ethanol and proteinase K and 80 for molecular index barcodes) assessed in this study.

Table 12. Interfering substance evaluated.

Substances	Level	# Samples	# Replicates/Sample
No Interferent	–	5	2
Melanin	0.025 µg/mL	5	2
Melanin	0.05 µg/mL	5	2
Melanin	0.1 µg/mL	5	2
Melanin	0.2 µg/mL	5	2
Proteinase K	0.04 mg/mL	5	2
Proteinase K	0.08 mg/mL	5	2
Ethanol	5%	5	2
Ethanol	2.5%	5	2
MIB	0	5	4
MIB	5%	5	4
MIB	15%	5	4
MIB	30%	5	4

Substances were considered as non-interfering if, when compared to no interferent, the DNA yield is sufficient to meet the standard processing requirements of DNA isolation (≥ 55 ng), if the quality was sufficient to create products per the specification of library construction (≥ 545 ng) and hybrid capture (≥ 140 ng), and the sample success rate (fraction of samples that met all process requirements and specifications), across all replicates in aggregate, is $\geq 90\%$. Sequence analysis was assessed as percent agreement for each sample and calculated as the number of replicates with the correct alteration call reported per the total number of replicates processed. Percent agreement (fraction of correct calls) was computed across all replicates. The acceptance for concordance required a minimum of 90% of correct calls within each treatment category.

All samples tested at all interfering substance levels met all process requirements and specifications; achieving the acceptance criterion of $\geq 90\%$, indicating that the sample quality was not impacted by the interfering substances at the levels evaluated. The concordance of variants for the melanin, proteinase K and MIB evaluations was 100%, and was 95.3% for the ethanol evaluation, each meeting the acceptance criterion of $\geq 90\%$, indicating that the performance was not affected by the tested interferents. In addition to the variants selected to represent specific alteration types summarized in Table 11, samples included in the study harbored 54 additional short alterations (substitutions and indels) and were 100% concordant across all replicates for each variant.

See Summary of Safety and Effectiveness Data for P160018 for additional interference studies, wherein the interference of necrotic tissue, triglycerides, hemoglobin, and xylene, in addition to ethanol, proteinase K, and MIBs, was evaluated in ovarian tissue and assessed *BRCA1/2* alterations.

An additional study was performed to assess the impact of endogenous and exogenous contaminants including melanin, ethanol, proteinase K, and MIB, on TMB-H (≥ 10 mutations per megabase) calling as a qualitative biomarker. The analysis included 19 retrospective samples from 3 previous studies and all acceptance criteria were met.

2.5.2 *In silico* Analysis – Hybrid Capture Bait Specificity

Bait specificity was addressed through an assessment of coverage at the base level for targeted regions included in F1CDx. Lack of bait specificity and/or insufficient bait inclusion would result in regions of diminished high quality mapped reads due to the capture of off-target content. This analysis showed that all regions that may harbor alterations associated with companion diagnostic claims consistently have high quality (MQS ≥ 30), deep coverage $\geq 250X$. When assessing the entire gene set, 99.45% of individual bases in targeted coding regions +/-2 bp of flanking intronic splice site are covered with $\geq 100X$ coverage, and 91.45% of individual bases within targeted introns platform-wide had $\geq 100X$ coverage.

2.5.3 Carryover/Cross-contamination

No carryover or cross-contamination was observed when alternating positive and negative samples for *BRCA1* and *BRCA2* variants, assessed in a checker-board pattern (see Summary of Safety and

Effectiveness Data for P160018). In addition, data from plates with high-level confirmed *ERBB2* amplifications, *EGFR* T790M alterations or *ALK* fusions were examined for cross-contamination in adjacent wells containing confirmed negative samples. No contamination was observed.

2.6 Precision: Repeatability and Reproducibility

Repeatability and reproducibility of alterations associated with CDx claims and platform-wide alterations, including agreement for MSI, TMB, and MAF of short variants, were evaluated. Repeatability between intra-run aliquots (run on the same plate under the same conditions) and reproducibility of inter-run aliquots (run on different plates under different conditions) were assessed and compared across three different sequencers and three different reagent lots, across multiple days of performance by multiple operators.

A total of 163 samples had alterations representative of CDx associated alterations as well as exemplar alterations in a variety of genomic contexts, as shown in Tables 13 and 14 below. Each sample also included additional alterations that were included in the assessment. The maximum insertion length in this study was 30 bp and the longest deletion was 263 bp.

Table 13. Sample set selection for CDx validation.

Gene or Biomarker	Number of Unique Samples	Alteration	Tumor Type
<i>EGFR</i>	3	Exon 19 Deletion	NSCLC
	2	Exon 21 L858R	
	2	Exon 20 T790M	
<i>KRAS</i>	3	Codons 12/13 substitution	CRC
<i>ALK</i>	3	Fusion	NSCLC
<i>BRAF</i>	3	V600E/V600K	Melanoma
<i>ERBB2</i>	3	Amplification	Breast cancer
<i>PIK3CA</i>	3 ¹	E545K/H1047R/H1047L	Breast cancer
<i>FGFR2</i>	5 ²	FGFR2 Fusions and rearrangement ³	Cholangiocarcinoma (CCA)
<i>MET</i>	8 ⁴	SNVs and indels that lead to Exon 14 skipping	NSCLC
HRR Genes	47	Base Substitutions, Indels, Rearrangements, Homozygous Deletions	Prostate
TMB	46 ⁴	TMB ≥ 10 mutations per megabase	Solid tumors
<i>NTRK1</i> <i>NTRK2</i> <i>NTRK3</i>	7 ⁴	Fusions	Solid tumors ⁵

¹Two samples are from the 47 samples originally included in the PMA precision study. An additional sample was analyzed in a subsequent precision study.

²Included 3 samples that included 24 replicates (2 runs x 2 replicates x 2 reagent lots x 3 sequencers), and two samples that included 36 replicates (2 runs x 3 replicates x 2 reagent lots x 3 sequencers)

³The precision study included *FGFR2-BICC1*, *FGFR2-CCDC6* fusion; *FGFR2-TFCP2* fusion, and an intron 17 rearrangement (no partner)

⁴The precision study included 7 samples with CDx *NTRK1/2/3* fusion positive status: Four (4) *NTRK3-EVT6* fusions, one (1) *NTRK1-TPM3* fusion, one (1) *NTRK1-LMNA* fusion, and one (1) *NTRK2-DSTYK* fusion.

⁵24 replicates performed (2 runs x 2 replicates x 2 reagent lots x 3 sequencers)

Table 14. Sample set selection for platform validation.

Alteration Type	Number of Unique Samples	Alteration Size	Genomic Context
Substitution	3	-	-
Short Insertion	2	1-2bp	Homopolymer Repeats
Short Insertion	2	1-2bp	Dinucleotide Repeats
Short Insertion	2	3-5bp	-
Short Insertion	2	>5bp	-

Alteration Type	Number of Unique Samples	Alteration Size	Genomic Context
Short Deletion	2	1-2bp	Homopolymer Repeats
Short Deletion	2	1-2bp	Dinucleotide Repeats
Short Deletion	2	3-5bp	-
Short Deletion	2	>5bp	-
Amplification	3	-	-
Homozygous Deletion	3	-	-
Rearrangement	3	-	-

Note: Two samples with *PIK3CA* alterations (E545K and H1047R) were represented in both the CDx and platform validation.

The results demonstrated that the F1CDx is robust regarding the repeatability and reproducibility of calling genomic alterations. Across all samples, the pre-sequencing process failure is 1.5%, and the no call rate is 0.18% for MSI, 6.38% for TMB (all) and 0.22% for TMB (>10 mut/Mb). Within the assessment of repeatability and reproducibility for CDx variants, all variants from all samples were 100% concordant. Percent of negative calls at each CDx variant location for wild-type samples was 100%.

Similarly, the platform-level repeatability and reproducibility showed high overall agreement across alteration bins, and high sample-level positive and negative call rates as summarized in Tables 15 and 16 below. The platform-level study included a total of 443 substitutions, 188 indels, 55 copy number amplifications, 13 copy number loss, and 18 rearrangements in the variant set across the samples.

Table 15. Reproducibility across variant bins (copy number, rearrangement, substitution, indels).

Variant Bin	# of Variants	# of valid Comparisons	# of Agreements	Positive Percent Agreement	95% CI Lower Limit	95% CI Upper Limit
CNAs	68	67,524	67,300	99.67%	99.62%	99.71%
Rearrangements	18	17,874	17,851	99.87%	99.81%	99.92%
Substitutions	443	439,899	439,649	99.94%	99.94%	99.95%
Indels	188	186,684	186,319	99.80%	99.78%	99.82%
All Variants	717	711,981	711,119	99.88%	99.87%	99.89%

Table 16. Positive and negative call rates per sample for platform variants (N=717).

Alteration Type(s) Assessed	exact 95% CI			exact 95% CI		
	PC Rate*	Lower	Upper	NC Rate**	Lower	Upper
CNA/RE/SUB	100.00%	99.40%	100.00%	99.98%	99.95%	99.99%
CNA/ SUB/Indel	99.37%	98.38%	99.83%	99.96%	99.92%	99.98%
SUB/Indel	100.00%	99.10%	100.00%	99.97%	99.95%	99.99%
CNA/ SUB/Indel	97.84%	96.89%	98.56%	99.84%	99.78%	99.89%
SUB/Indel	99.81%	98.94%	100.00%	99.98%	99.95%	99.99%
SUB/Indel	99.60%	97.81%	99.99%	99.94%	99.90%	99.97%
CNA/ SUB/Indel	98.33%	97.11%	99.14%	99.98%	99.96%	100.00%
SUB/Indel	100.00%	99.83%	100.00%	99.97%	99.94%	99.99%
CNA/ SUB/Indel	100.00%	99.32%	100.00%	99.98%	99.96%	100.00%
RE/ SUB/Indel	96.46%	94.14%	98.05%	99.96%	99.92%	99.98%
CNA/ SUB	98.67%	97.27%	99.46%	99.98%	99.96%	100.00%
CNA/RE/SUB/Indel	96.27%	95.39%	97.02%	99.87%	99.82%	99.91%
RE/SUB/Indel	98.23%	97.48%	98.80%	99.66%	99.58%	99.73%
CNA/ SUB/Indel	98.32%	97.57%	98.89%	99.92%	99.88%	99.95%
SUB/Indel	99.30%	98.90%	99.58%	99.90%	99.86%	99.94%
CNA/RE/SUB/Indel	85.42%	82.27%	88.20%	99.89%	99.84%	99.93%
RE/SUB/Indel	97.75%	96.42%	98.68%	99.98%	99.95%	99.99%
RE/SUB/Indel	95.30%	92.97%	97.03%	99.96%	99.93%	99.98%
CNA/RE/SUB/Indel	100.00%	98.31%	100.00%	99.89%	99.84%	99.93%
CNA/RE/SUB/Indel	100.00%	99.25%	100.00%	99.96%	99.93%	99.98%

Alteration Type(s) Assessed	exact 95% CI		NC Rate**	exact 95% CI		
	PC Rate*	Lower		Upper	Lower	Upper
CNA /SUB	96.83%	94.90%	98.17%	99.94%	99.90%	99.97%
CNA/RE/SUB/Indel	95.97%	94.06%	97.40%	99.98%	99.96%	100.00%
CNA/ SUB/Indel	100.00%	99.42%	100.00%	99.93%	99.89%	99.96%
CNA/RE/SUB/Indel	100.00%	99.30%	100.00%	99.95%	99.91%	99.97%
RE/SUB	100.00%	99.05%	100.00%	100.00%	99.98%	100.00%
CNA /SUB	96.99%	95.39%	98.15%	99.84%	99.79%	99.89%
CNA/RE/SUB/Indel	100.00%	98.95%	100.00%	99.93%	99.89%	99.96%
CNA/RE/SUB/Indel	99.80%	99.29%	99.98%	99.98%	99.96%	100.00%

*Abbreviations: SUB=substitution, Indel=Insertion or Deletion, CNA=Copy Number Alteration, RE=Rearrangement, PC=Positive Call, NC=Negative Call

For the assessment of MSI, 100% agreement was observed, with a lower limit of 99.7% and upper limit of 100%. For TMB determination, thirteen samples met the inclusion criteria (TMB \geq 10) for assessment of repeatability and reproducibility. Twelve of 13 samples (92.3%) met the \leq 20% Coefficient of Variation (CV) requirements; one sample fell just outside this requirement with a repeatability CV of 21% and reproducibility CV of 23%. The putative source of variability was determined to be low depth of coverage for this sample.

A supplementary analysis was conducted to evaluate the intermediate precision for demonstrating the repeatability and reproducibility in detecting TMB-H status (\geq 10 mutations per megabase) as a CDx biomarker in 46 pan tumor FFPE specimens. Repeatability and reproducibility results are 99.54% (95% CI [98.39%, 99.89%]) and 99.72% (95% CI [99.18%, 99.94%]), respectively, for the TMB cut-off of 10 mutations per megabase.

2.6.1 Reagent Lot-to-Lot Reproducibility

Three lots of critical reagents were assessed for four replicates per sample in a full factorial design. Reagents were evaluated as internally prepared kits for each process step (LC, HC, sequencing). The use of three different lots of reagents did not impact performance. Twenty-seven of 28 samples (96.4%) had pairwise agreement estimates (APA and ANA) above 95%; one sample had APA estimates below 90% (85.9% to 88.7%). ANA estimates were greater than 99%. The putative source of variability was determined to be non-focal copy number amplifications with low copy number close to the calling threshold observed in one sample; no specific reagent lot performed differently among three lots for this sample.

2.6.2 Instrument-to-Instrument Reproducibility

Four replicates per sample were sequenced on each of three Illumina HiSeq4000 sequencers, serial numbers K00255, K00256, and K00257 in a full factorial design. The use of three different sequencers did not impact performance. Twenty-seven of 28 samples (96.4%) had pairwise agreement estimates (APA and ANA) at least 97%; one sample had APA estimates below 90% (86.6% to 89.2%). ANA estimates were greater than 99%. The putative source of variability was determined to be non-focal copy number amplifications with low copy number close to the calling threshold observed in one sample; no specific sequencer performed differently among three sequencers for this sample.

2.6.3 Site-to-Site Reproducibility

FMI performed a site-to-site precision study with the objective of evaluating repeatability and reproducibility of the F1CDx assay with challenging samples near the LoD across many tumor types. This study assessed the repeatability and reproducibility of the detection of alterations associated with CDx claims and other tumor profiling alterations. In addition, the study evaluated agreement for MSI, LOH and TMB calling. Repeatability between intra-run replicates (run on the same plate under the same conditions) and reproducibility of inter-run replicates (run on different plates under different conditions) were assessed and compared between the two FMI sites (Cambridge, MA and Morrisville, NC), two reagent lots, and three non-consecutive days. The study demonstrated repeatable and reproducible results across the CDx variants including:

NSCLC:

- *EGFR* exon 19 deletions, exon 21 L858R, exon 20 T790M
- *ALK* rearrangement
- *BRAF* V600E

Melanoma:

- *BRAF* V600E and V600K

Breast Cancer:

- *ERBB2* (HER2) amplification
- *PIK3CA* mutations

Colorectal Cancer:

- *KRAS* wild-type
- *NRAS* wild-type

Ovarian Cancer:

- *BRCA1/2*
- LOH

Solid Tumors:

- TMB-H (≥ 10 mutations per megabase)

In the assessment of other tumor profiling alterations, the study demonstrated repeatable and reproducible results with a multivariant analysis for all alteration types, as well as MSI. The totality of the results demonstrate that the F1CDx assay has robust performance with respect to repeatability and reproducibility in calling genomic alterations across two sites (i.e., Cambridge, MA and Morrisville, NC). In summary, comparable results for FMI Cambridge and FMI Morrisville were observed when detecting CDx variants (including LOH for ovarian cancer and TMB as a qualitative biomarker [≥ 10 mutations per megabase]), tumor profiling alterations, as well as genomic signatures (e.g., MSI).

2.7 Analytical Sensitivity: Limit of Detection (LoD) and Limit of Blank (LoB)

The Limit of Detection (LoD) of alterations assessed by FoundationOne[®]CDx (F1CDx) was evaluated. The LoDs of sixteen (16) CDx biomarkers are summarized in Tables 17-1 and 17-2 below. An additional twelve (12) categories of alteration types were evaluated for the F1CDx assay platform validation. FFPE tumor samples were selected for each of the variant categories. For each sample, six levels of MAF, with 13 replicates per level, were evaluated for a total of 78 replicates per sample. LoD for short variants, including substitutions and indels, is based on allele fraction. LoD for structural variants (fusions, amplifications, homozygous deletions, rearrangements) and TMB is based on computational tumor purity. Computational tumor purity is calculated by fitting the observed log-ratio and minor allele frequency data with statistical models that predict a genome-wide copy number profile, tumor ploidy, and tumor purity (i.e., computational tumor purity). The log-ratio profile is obtained by normalizing aligned tumor sequence reads by dividing read depth by that of a process-matched normal control, followed by a GC-content bias correction using Loess regression. The minor allele frequency profile is obtained from the heterozygous genome-wide SNPs. For platform-wide LoD assessment, the indels were grouped together (other than homopolymer repeat context) as they are similar in LoD characteristics. The indels ranged from 1 bp up to 42 bp insertions and deletions up to 276 bp. Indels at homopolymer repeat context had higher LoD, with a dependency on the length of the repeat context. In addition, LoD of MSI-H was also evaluated. The LoD for representative alterations detected by the F1CDx platform is summarized in Tables 18-1 and 18-2.

Table 17-1. Summary of LoD for alterations associated with CDx claims (short variants). LoD is based on Allele Fraction.

Alteration	LoD ¹ Allele Fraction (%) (95% Hit Rate)	LoD ² Allele Fraction (%) (Probit)
<i>EGFR</i> L858R	2.4%	< 2.4% (all detected)
<i>EGFR</i> Exon 19 deletion	5.1%	3.4%
<i>EGFR</i> T790M	2.5%	1.8%
<i>KRAS</i> G12/G13	2.3%	< 2.3% (all detected)
<i>BRAF</i> V600E/K	2.0%	< 2.0% (all detected)
<i>MET</i> Exon 14 SNVs ³	N/A	< 2.9% (all detected)
<i>MET</i> Exon 14 insertion and deletion ³	N/A	5.7%
<i>PIK3CA</i> E542K	4.9%	Not Calculated
<i>BRCA1/2</i>⁴ Alteration in non-repetitive or homopolymer <4 bp	N/A	5.9%
Deletion in 8 bp homopolymer	N/A	15.3%
HRR gene base substitutions	5.44% - 6.33% ⁵	Not calculated
HRR gene indels	5.22% - 12.74% ⁵	Not calculated

¹ LoD calculations for the CDx variants were based on the hit rate approach, as there were less than three levels with hit rate between 10% and 90% for all CDx variants (not including *BRCA1/2* variants). LoD from the hit rate approach is defined as the lowest level with 95% hit rate (worst scenario).

² LoD calculations for the CDx variants based on the probit approach with 95% probability of detection.

³ For each sample, five levels of MAF, with 10 replicates per level, were evaluated for a total of 50 replicates per sample.

⁴ See Summary of Safety and Effectiveness Data for P160018.

⁵ LoD defined as the lowest level with 95% hit rate or greater.

Table 17-2. Summary of LoD (C95) based on tumor purity for biomarkers associated with CDx claims.

Alteration	Tumor Purity (%) (95% Hit Rate) ¹	Tumor Purity (%) (Probit) ²
<i>ALK</i> fusion	2.6% ³	1.8%
<i>ERBB2</i> amplification	25.3% ⁴	19.7%
<i>BRCA2</i> homozygous deletion (HD)	8.8% ⁵	Not Calculated
LOH ⁶	35%	30%
<i>FGFR2</i> fusions	5.31% ⁷	5.38%
HRR gene rearrangements ⁸	20.1% ⁷	Not Calculated
HRR gene homozygous deletions ⁸	23.9% ⁷	Not Calculated
TMB ≥ 10 mutations per megabase ⁸	28.16% ⁷	Not Calculated
<i>NTRK1</i> fusions ^{9,10}	12.10%	N/A
<i>NTRK2</i> fusions ^{9,11}	11.5%	N/A
<i>NTRK3</i> fusions ^{9,12}	6.1%	N/A

¹ Sensitivity calculations for the CDx variants were based on the hit rate approach, as there were less than three levels with hit rate between 10% and 90%. LoD from the hit rate approach is defined as the lowest level with 95% hit rate (worst scenario).

² Sensitivity calculations for the CDx variants based on the probit approach with 95% probability of detection.

³ The number of chimeric reads for the sample evaluated is 16 at the indicated tumor fraction.

⁴ The number of copy number amplifications for the sample evaluated is 6 at the indicated tumor fraction.

⁵ The LoD calculation for the *BRCA2* HD was based on the hit rate approach, as there was a hit at every dilution level tested, making the probit regression not applicable.

⁶See Summary of Safety and Effectiveness Data for P160018/S001.

⁷Calculated using the 95% hit rate.

⁸For each sample, five levels of tumor purity, with 20 replicates per level except for the highest level at which 14 replicates were tested, were evaluated for a total of 94 replicates per sample.

⁹For each sample, a total of 94 tumor dilution replicates were assessed, including twenty (20) replicates for each level of tumor purity, excluding the highest level, for which only fourteen (14) replicates were performed.

¹⁰ The LoD study included 2 samples with CDx *NTRK1* fusion positive status: one (1) *NTRK1-LMNA* fusion, and one (1) *NTRK1-TRP* fusion.

¹¹ The LoD study included 2 samples with CDx *NTRK2* fusion positive status: one (1) *NTRK2-BCR* fusion, and one (1) *NTRK2-GARNL3* fusion.

¹² The LoD study included 3 samples with CDx *NTRK3* fusion positive status: three (3) *NTRK3-EVT6* fusions.

N/A=not applicable.

Table 17-3. Summary of analytical sensitivity based on reads for biomarkers associated with CDx claims

Alteration	Reads (95% Hit Rate) ¹
<i>NTRK1</i> fusions	24.55
<i>NTRK2</i> fusions	24.16
<i>NTRK3</i> fusions	14.65

¹Sensitivity calculations for the CDx variants were based on the hit rate approach, as there were less than three levels with hit rate between 10% and 90%. LoD from the hit rate approach is defined as the lowest level with 95% hit rate.

Table 18-1. Summary of representative LoD for F1CDx platform (short variants).

Variant Category	Subcategory	N	Range LoD ¹ Allele Fraction (%)
Base Substitutions	known ³	21 ²	1.8-7.9 ²
	other ⁴	166	5.9-11.8
Indels at non-homopolymer context, including insertions up to 42bp and deletions up to 276bp	Known	3	4.5-6.5
	Other	17	6.0-10.2
Indels at homopolymer context	5bp repeat	8	10.0-12.2
	6bp repeat	2	13.6-13.7
	7bp repeat	4	16.3-20.4
	8bp repeat	3	17.0-20.0

¹LoD calculations for the platform variants were based on the hit rate approach for variants with less than three levels with hit rate between 10% and 90% and probit approach for variants with at least three levels with hit rate between 10% and 90%. LoD from the hit rate approach is defined as the lowest level with 100% hit rate (worst scenario).

²Data includes an alteration in the *TERT* promoter, 124C>T (LoD of 7.9%). *TERT* is the only promoter region interrogated and is highly enriched for repetitive context of poly-Gs, not present in coding regions.

³Alterations classified as "known" are defined as those that are listed in COSMIC

⁴Alterations classified as "other" include truncating events in tumor suppressor genes (splice, frameshift and nonsense) as well as variants that appear in hotspot locations but do not have a specific COSMIC association, or are considered variants of unknown significance (VUS) due to lack of reported evidence and conclusive change in function.

Table 18-2. Summary of representative analytical sensitivity for tumor purity for F1CDx platform alterations (copy number variants and rearrangements).

Variant Category	N	Range Tumor Purity (%) ¹
Copy Number Amplifications (CN>10)	8	9.6%-18.5%
Copy Number Amplifications (6≤CN≤10)	7	19.5%-58.3% ²
Copy Number: Homozygous Deletions	3	33.4%-33.4%
Genomic Rearrangements	3	9.2%-14.9%

MSI-High	3	8.3%-15.8%
----------	---	------------

¹Sensitivity calculations for the platform variants were based on the hit rate approach for variants with less than three levels with hit rate between 10% and 90% and probit approach for variants with at least three levels with hit rate between 10% and 90%. LoD from the hit rate approach is defined as the lowest level with 100% hit rate (worst scenario)

²Max represents VUS alteration at calling threshold.

The LoB of zero was confirmed through the assessment of alterations within the LoB samples, with a percentage of false-positive results less than 5% (type I error risk $\alpha=0.05$). Seventy-five (75) samples were used for the assessment of LoB. For all the alterations evaluated for LoD, the LoB of zero was confirmed. A similar study was conducted for *BRCA1/2* alterations (PMA P160018) with no false-positive *BRCA* calls observed, thus confirming the LoB of zero for *BRCA*. An additional study was conducted for TMB in twenty-one (21) samples with no false positive TMB-H calls (≥ 10 mutations per megabase) observed, thus confirming the LoB of zero for TMB.

2.8 Stability

2.8.1 Reagent Stability

Identical reagents with the same specifications are used following the same protocols for both the FoundationFocus CDx_{BRCA} Assay and FoundationOne[®]CDx (F1CDx). For reagent stability performance data, see the Summary of Safety and Effectiveness Data for P160018. The claimed reagent stability is 4 months for the library construction (LC) and hybrid capture (HC) kits, and 3 months for the sequencing kits.

2.8.2 DNA Stability

Stability of DNA was evaluated through a retrospective review of data generated using the FoundationOne LDT assay. Samples from 47 unique clinical specimens from 21 different tissues of origin were evaluated. The sample set covered 200 alterations inclusive of nucleotide changes, indels, copy number amplifications, copy number losses and rearrangements. Duration of DNA storage at time of testing ranged from 48 to 464 days, with a median of 184 days and a mean of 199 days. A total of 199 of 200 alteration calls were concordant. A 242-day old sample with a single alteration call that met inclusion criteria was discordant; however, this sample was classified as not meeting all QC criteria due to other data quality issues. DNA age for the sample with discordance was 242 days. Sixteen other samples had concordant calls with DNA age >242 days. Based on these data, DNA stored in accordance with internal procedures can be stored at 4°C for up to 6 weeks and -20°C for 5 months. Further supporting this retrospective data is a prospective study conducted using ovarian cancer samples, see the Summary of Safety and Effectiveness Data for P160018. An additional prospective DNA stability study is underway.

2.8.3 FFPE Sample Stability

The FFPE Slide Stability Study is an ongoing study with data summarized for T₀, T₁ (30 days), and T₂ (6 months). This study evaluated the stability of FFPE tumor tissue prepared as slides prior to DNA extraction for use within the FoundationOne[®]CDx (F1CDx) assay. Five tumor samples including ovarian, lung, colorectal cancer, melanoma and breast cancer that contained a variety of DNA alterations, as described in Table 19 below. The five samples were selected to include specific alteration types that were reflective of the CDx alterations, but were found to contain additional alterations as well (13 CNAs, one rearrangement, 53 base substitutions and five indels; refer to Table 20). To assess stability of pre-cut FFPE tissue for genomic alterations, the agreement between results from the defined time points for each sample were calculated by comparing the alteration call reported at each follow-up time point to the alteration call at baseline (T₀). Alterations at the 30-day time point and the 6-month time point are in 100% agreement with the day 0 baseline results (T₀). The FFPE slides are considered stable for at least 6 months. Further assessment at months 12 and 15 will evaluate stability of FFPE slides beyond 6 months.

Table 19. Stability results at baseline, 30 days and 6 months.

Tissue	Baseline Call (T ₀)		Percent Agreement to T ₀	Percent Agreement to T ₀
	Gene	Variant Effect	30 days (T ₁)	6 months (T ₂)
Ovarian	<i>BRCA1</i>	c.1340_1341insG, p.H448fs*8	100% (2/2)	100% (2/2)

Tissue	Baseline Call (T ₀)		Percent Agreement to T ₀	Percent Agreement to T ₀
	Gene	Variant Effect	30 days (T ₁)	6 months (T ₂)
Lung	<i>KRAS</i>	c.34G>T, p.G12C	100% (2/2)	100% (2/2)
CRC	<i>PIK3CA</i>	c.3139C>T, p.H1047Y	100% (2/2)	100% (2/2)
CRC	<i>PIK3CA</i>	c.1258T>C, p.C420R	100% (2/2)	100% (2/2)
Melanoma	<i>CDKN2A</i>	Homozygous Deletion	100% (2/2)	100% (2/2)
Melanoma	<i>CDKN2B</i>	Homozygous Deletion	100% (2/2)	100% (2/2)
Breast	<i>ERBB2</i>	Amplification	100% (1/1)	100% (2/2)

Table 20. Percent agreement for each variant type.

Variant type	Number of variants	30 days (T ₁) Percent Agreement (# agreement/total)	95% 2-sided CI LB, UB*	6 months (T ₂) Percent Agreement (# agreement/total)	95% 2-sided CI LB, UB*
Copy Number	13	100% (23/23)	85.2%, 100.0%	100% (26/26)	86.8%, 100.0%
Rearrangement	1	100% (2/2)	15.8%, 100.0%	100% (2/2)	15.8%, 100.0%
Substitution	53	100% (98/98)	96.3%, 100.0%	100% (106/106)	96.6%, 100.0%
Insertion/Deletion	5	100% (7/7)	59.0%, 100.0%	100% (10/10)	69.2%, 100.0%

*LB: lower bound; UB: upper bound

2.9 Reagent Lot Interchangeability

Identical reagents with the same specifications are used following the same protocols for both the FoundationFocus CD_XBRCA assay and FoundationOne[®]CDx. For reagent lot interchangeability performance data, see the Summary of Safety and Effectiveness Data for P160018.

2.10 General Lab Equipment and Reagent Evaluation

2.10.1 DNA Amplification

Identical reagents and equipment with the same specifications are used following the same protocols for both the FoundationFocus CD_XBRCA Assay and FoundationOne[®]CDx. For DNA amplification performance data, see the Summary of Safety and Effectiveness Data for P160018.

2.10.2 DNA Extraction

The performance of DNA extraction from FFPE tumor specimens was evaluated. The DNA extraction procedure for the FoundationOne[®]CDx (F1CDx) assay was assessed by testing FFPE specimens including two samples per tissue type for ten different tumor tissue types including lung, breast, ovarian, melanoma, colorectal, brain, hepatic, pancreatic, thyroid, and bladder with different representative types of alterations. Samples were run in duplicate for a total of 240 extractions, employing two different KingFisher Flex Magnetic Particle Processors (120 extractions per processor) and comparing across three extraction reagent lots (80 extractions per reagent lot). Average DNA yield was calculated across twelve (12) replicates for each sample. All average DNA yields were significantly above the minimum requirement of 55 ng, with the minimum being 758.3 ng. Only one sample aliquot of the 240 replicates failed the DNA yield specification, and the success rates based on the reagent lot and the equipment were 98.8% (79/80) and 99.2% (119/120), respectively, passing the acceptance criteria (≥90%). Concordance of all genomic alterations detected was also analyzed for all variants across 12 replicates for each sample. Table 21 provides a summary of concordance across replicates. A study with an additional ten samples will be completed post-market.

Table 21. Summary of concordance across replicates of DNA extraction study.

Group	N _{concordance}	N _{total}	Concordance	95% CI
Substitutions (All MAF)	2700	2969	90.9%	[89.9% 91.9%]
Substitutions (MAF > 10%)	1631	1637	99.6%	[99.2% 99.9%]
Substitutions (All MAF, excluding hypermutated sample)*	1663	1685	98.7%	[98% 99.1%]
Indel (All)	465	476	97.7%	[95.9% 98.8%]
Copy Number: Amplification	307	314	97.8%	[95.4% 99%]

Copy Number: Loss	132	144	91.7%	[85.9% 95.3%]
Rearrangement	84	90	93.3%	[85.9% 97.2%]

*One sample included in the study was hypermutated, harboring many alterations near LoD and exhibited evidence of external contamination. Concordance of substitutions was 80.8% for this sample.

A DNA extraction study was performed to evaluate the FoundationOne[®]CDx (F1CDx) assay DNA extraction procedure with respect to TMB-H (≥ 10 mutations per megabase) calling. The analysis included 35 retrospective samples and all acceptance criteria were met.

2.11 Guard banding/Robustness

Guard banding studies were performed to evaluate the impact of process variation with regard to the measurement of DNA concentration at various stages of the process. Guard bands were evaluated relative to observed and measured process variability for Library Construction (LC), Hybrid Capture (HC), and Sequencing. Each of the three guard banding experiments demonstrated reliable and robust performance at all DNA input levels evaluated.

A total of 255 samples were processed; ninety (90) to assess DNA input into LC, ninety (90) to assess DNA input into HC, and seventy-five (75) to assess DNA input into sequencing. For LC input, five samples were run in triplicate over six different DNA input levels representing -20% and -50% from the lower limit (50 ng) to +20% and +50% from the upper limit (1000 ng) needed for LC (n=90). Five samples were run in triplicate over six DNA input levels representing -25% and -50% from the lower limit (0.5 μ g) to +25% and +50% from the upper limit (2.0 μ g) for HC input. The third component of the guard banding study evaluated the captured DNA input into the sequencing reaction. Five samples were run in triplicate over five different DNA input levels representing $\pm 10\%$ and $\pm 20\%$ from the required amount needed for sequencing (1.75 nM; n=75). Concordance of detected alterations was calculated for each condition across successful replicates. Results from this study support the robustness of the FoundationOne[®]CDx (F1CDx) process. The study design and results are shown below in Tables 22-1 through 22-4.

Table 22-1. Summary of the success rate per process and per input level, and concordance of substitutions (SUB) among successful replicates.

Process	Input Level	# of Sample Failures	Variant Type	# of Concordant Successes	# of Variant Comparisons	Success Rate (95% CI) (Number of Concordant comparisons)
LC	25 ng	1/15	SUB	184	184	100.0% (98.0%, 100.0%)
LC	40 ng	0/15	SUB	192	192	100.0% (98.1%, 100.0%)
LC	50 ng	0/15	SUB	191	192	99.5% (97.1%, 100%)
LC	1000ng	0/15	SUB	192	192	100.0% (98.1%, 100.0%)
LC	1200 ng	0/15	SUB	191	192	99.5% (97.1%, 100%)
LC	1500 ng	0/15	SUB	190	192	99.0% (96.3%, 99.9%)
HC	0.25 μ g	15/15	SUB	0	0	NA* (no samples sequenced)
HC	0.375 μ g	12/15	SUB	30	30	100.0% (88.4%, 100.0%)
HC	0.5 μ g	1/15	SUB	166	166	100.0% (97.8%, 100.0%)
HC	2.0 μ g	0/15	SUB	192	192	100.0% (98.1%, 100.0%)
HC	2.5 μ g	0/15	SUB	192	192	100.0% (98.1%, 100.0%)
HC	3.0 μ g	0/15	SUB	192	192	100.0% (98.1%, 100.0%)
Seq	1.4 nM	0/15	SUB	192	192	100.0% (98.1%, 100.0%)
Seq	1.575 nM	1/15	SUB	180	180	100.0% (98.0%, 100.0%)
Seq	1.75 nM	1/15	SUB	184	184	100.0% (98.0%, 100.0%)
Seq	1.925 nM	0/15	SUB	192	192	100.0% (98.1%, 100.0%)

Process	Input Level	# of Sample Failures	Variant Type	# of Concordant Successes	# of Variant Comparisons	Success Rate (95% CI) (Number of Concordant comparisons)
Seq	2.1 nM	0/15	SUB	192	192	100.0% (98.1%, 100.0%)

* All samples failed at the input level of 0.25 µg and as a result, there is no data available to present for that level.

Table 22-2. Summary of the success rate per process and per input level, and concordance of insertions and deletions (INDEL) among successful replicates.

Process	Input Level	# of sample failures	Variant Type	# of concordant successes	# of variant comparisons	Success Rate (95% CI) (Number of Concordant comparisons)
LC	25 ng	1/15	INDEL	17	17	100.0% (80.5%, 100.0%)
LC	40 ng	0/15	INDEL	18	18	100.0% (81.5%, 100.0%)
LC	50 ng	0/15	INDEL	18	18	100.0% (81.5%, 100.0%)
LC	1000ng	0/15	INDEL	18	18	100.0% (81.5%, 100.0%)
LC	1200 ng	0/15	INDEL	18	18	100.0% (81.5%, 100.0%)
LC	1500 ng	0/15	INDEL	18	18	100.0% (81.5%, 100.0%)
HC	0.25 µg	15/15	INDEL	0	0	NA* (no samples sequenced)
HC	0.375 µg	12/15	INDEL	4	4	100.0% (39.8%, 100.0%)
HC	0.5 µg	1/15	INDEL	18	18	100.0% (81.5%, 100.0%)
HC	2.0 µg	0/15	INDEL	18	18	100.0% (81.5%, 100.0%)
HC	2.5 µg	0/15	INDEL	18	18	100.0% (81.5%, 100.0%)
HC	3.0 µg	0/15	INDEL	18	18	100.0% (81.5%, 100.0%)
Seq	1.4 nM	0/15	INDEL	18	18	100.0% (81.5%, 100.0%)
Seq	1.575 nM	1/15	INDEL	16	16	100.0% (79.4%, 100.0%)
Seq	1.75 nM	1/15	INDEL	17	17	100.0% (80.5%, 100.0%)
Seq	1.925 nM	0/15	INDEL	18	18	100.0% (81.5%, 100.0%)
Seq	2.1 nM	0/15	INDEL	18	18	100.0% (81.5%, 100.0%)

* All samples failed at the input level of 0.25 µg and as a result, there is no data available to present for that level.

Table 22-3. Summary of the success rate per process and per input level, and concordance of rearrangements (RE) among successful replicates.

Process	Input Level	# of sample failures	Variant Type	# of concordant successes	# of variant comparisons	Success Rate (95% CI) (Number of Concordant comparisons)
LC	25 ng	1/15	RE	6	6	100.0% (54.1%, 100.0%)
LC	40 ng	0/15	RE	6	6	100.0% (54.1%, 100.0%)
LC	50 ng	0/15	RE	6	6	100.0% (54.1%, 100.0%)
LC	1000ng	0/15	RE	6	6	100.0% (54.1%, 100.0%)
LC	1200 ng	0/15	RE	6	6	100.0% (54.1%, 100.0%)
LC	1500 ng	0/15	RE	6	6	100.0% (54.1%, 100.0%)
HC	0.25 µg	15/15	RE	0	0	NA* (no samples sequenced)
HC	0.375 µg	12/15	RE	2	2	100.0% (15.8%, 100.0%)
HC	0.5 µg	1/15	RE	6	6	100.0% (54.1%, 100.0%)
HC	2.0 µg	0/15	RE	6	6	100.0% (54.1%, 100.0%)
HC	2.5 µg	0/15	RE	6	6	100.0% (54.1%, 100.0%)
HC	3.0 µg	0/15	RE	6	6	100.0% (54.1%, 100.0%)

Process	Input Level	# of sample failures	Variant Type	# of concordant successes	# of variant comparisons	Success Rate (95% CI) (Number of Concordant comparisons)
Seq	1.4 nM	0/15	RE	8	9	88.9% (51.8%, 99.7%)
Seq	1.575 nM	1/15	RE	9	9	100.0% (66.4%, 100.0%)
Seq	1.75 nM	1/15	RE	8	8	100.0% (63.1%, 100.0%)
Seq	1.925 nM	0/15	RE	8	9	88.9% (51.8%, 99.7%)
Seq	2.1 nM	0/15	RE	7	9	77.8% (40.0%, 97.2%)

* All samples failed at the input level of 0.25 µg and as a result, there is no data available to present for that level.

Table 22-4. Summary of the success rate per process and per input level, and concordance of copy number alterations (CN) among successful replicates.

Process	Input Level	# of sample failures	Variant Type	# of concordant successes	# of variant comparisons	Success Rate (95% CI) (Number of Concordant comparisons)
LC	25 ng	1/15	CN	128	128	100.0% (97.2%, 100.0%)
LC	40 ng	0/15	CN	132	132	100.0% (97.2%, 100.0%)
LC	50 ng	0/15	CN	132	132	100.0% (97.2%, 100.0%)
LC	1000ng	0/15	CN	132	132	100.0% (97.2%, 100.0%)
LC	1200 ng	0/15	CN	132	132	100.0% (97.2%, 100.0%)
LC	1500 ng	0/15	CN	132	132	100.0% (97.2%, 100.0%)
HC	0.25 µg	15/15	CN	0	0	NA* (no samples sequenced)
HC	0.375 µg	12/15	CN	13	14	92.9% (66.1%, 99.8%)
HC	0.5 µg	1/15	CN	107	108	99.0% (95.0 %, 100.0%)
HC	2.0 µg	0/15	CN	129	132	97.7% (93.5%, 99.5%)
HC	2.5 µg	0/15	CN	129	132	97.7% (93.5%, 99.5%)
HC	3.0 µg	0/15	CN	130	132	98.5% (94.6%, 99.8%)
Seq	1.4 nM	0/15	CN	131	132	99.2% (95.9%, 100.0%)
Seq	1.575 nM	1/15	CN	122	128	95.3% (90.1%, 98.3%)
Seq	1.75 nM	1/15	CN	128	128	100.0% (97.2%, 100.0%)
Seq	1.925 nM	0/15	CN	130	132	98.5% (94.6%, 99.8%)
Seq	2.1 nM	0/15	CN	131	132	99.2% (95.9%, 100.0%)

* All samples failed at the input level of 0.25 µg and as a result, there is no data available to present for that level.

3. Clinical Studies

Several CDx claims described in sections 3.1-3.6 and summarized in Section 3.7 were based on a non-inferiority (NI) statistical testing approach using the enrichment design presented in the paper by Li (2016)¹, when the concordance study sample is not a random sample from the companion diagnostic FoundationOne[®]CDx (F1CDx) intended use population and a reference standard is not available.

To assess clinical concordance, F1CDx was compared to FDA-approved CDxs (CCD). All studies based on NI passed the acceptance criteria specified in each study protocol. Clinical concordance studies, with the exception of *ALK* and *EGFR* T790M, were subject to pre-screening bias. Therefore, the concordance results may be over- or underestimated and the failure rate may be underestimated.

Additional CDx claims are described in sections 3.8-3.14 including:

- A concordance study between F1CDx and FoundationFocus CDx_{BRCA LOH} was conducted for the reporting of *BRCA1*, *BRCA2* and loss of heterozygosity (LOH) in ovarian cancer patients.

- For the CDx indication to identify *PIK3CA* alterations in breast cancer patients intended to be treated with alpelisib, the effectiveness of the F1CDx assay was demonstrated through the clinical bridging study using specimens from the patients screened for enrollment into the study CBYL719C2301 (SOLAR-1).
- For the CDx indication to identify *BRCA1* and *BRCA2* in ovarian patients intended to be treated with olaparib, the effectiveness was demonstrated using specimens from the patients screened for enrollment into study D0818C00001 (SOLO1).
- For the CDx indication to identify *FGFR2* fusions and select rearrangements in cholangiocarcinoma (CCA) patients to determine eligibility for treatment with pemigatinib, the effectiveness of F1CDx was demonstrated through a clinical bridging study using specimens from the patients screened for enrollment into the INCB 54828-202 (FIGHT-202) trial.
- For the indication to identify SNVs and indels that lead to *MET* exon 14 skipping in NSCLC patients to determine eligibility for treatment with capmatinib, the effectiveness of the F1CDx was demonstrated through a clinical bridging study using specimens from the patients screened for enrollment into the CINC280A2201 (GEOMETRY-mono 1) trial.
- For the CDx indication to identify mutations in homologous recombination repair (HRR) genes in metastatic castration-resistant prostate cancer (mCRPC) patients to determine eligibility for treatment with olaparib, the effectiveness of the F1CDx assay was demonstrated based on the results from the PROfound trial.
- For the CDx indication to identify solid cancer patients with TMB-H (defined as ≥ 10 mutations per megabase) tumors to determine eligibility for treatment with pembrolizumab, the effectiveness of the F1CDx assay was demonstrated through a prospectively-planned retrospective analysis of clinical specimens from the patients enrolled in the KEYNOTE-158 clinical trial.
- For the CDx indication to identify *NTRK1*, *NTRK2*, or *NTRK3* fusions in patients with solid tumors that are intended to be treated with larotrectinib, the effectiveness of the F1CDx assay was demonstrated through the clinical bridging study using specimens from patients enrolled in the LOXO-TRK-14001 (Bayer 20288, NCT02122913), -15002 (Bayer 20289, NAVIGATE, NCT02576431), and -15003 (Bayer 20290, SCOUT, NCT02637687) clinical trials.

3.1 FoundationOne®CDx Concordance Study for *EGFR* Exon19del/L858R

Clinical validity of FoundationOne®CDx (F1CDx) as a companion diagnostic used for identifying patients with advanced NSCLC who may be eligible for treatment with Gilotrif® (afatinib), Iressa® (gefitinib), or Tarceva® (erlotinib) was established by retrospectively testing 282 samples from NSCLC patients. The *EGFR* diagnostic results from the F1CDx assay were compared against those obtained from the approved **cobas**® *EGFR* Mutation Test v2 (Roche Molecular Systems, referred to as **cobas**® *EGFR* v2 below). Samples were tested using **cobas**® *EGFR* v2 (CCD1) with an approximately equal number of mutation positive and negative samples, followed by testing with F1CDx and a second, replicate testing of **cobas**® *EGFR* v2 (CCD2). NSCLC tumor samples used for this study were not obtained from a clinical trial and had limited demographic data available. For this study age and gender data were available and were found to be similar to the pivotal study EURTAC.

Two separate concordance analyses were performed: one with samples with complete records only (N = 267), and the other with all the 282 samples, where missing data were handled by multiple imputation. Data from concordance testing are summarized in Table 23 below.

Table 23. Concordance Table with CCD1, CCD2 and F1CDx results with eligible samples.

	CCD1+				CCD1-			
	CCD2+	CCD2-	CCD2 missing	Total	CCD2+	CCD2-	CCD2 missing	Total
F1CDx+	106	0	0	106	1	1*	0	2
F1CDx-	2**	1	0	3	3	153	0	156

F1CDx Missing	3	0	0	3	1	9	2	12
Total	111	1	0	112	5	163	2	170

* QRF006212 was the only sample where both replicates of the **cobas**[®] EGFR v2 assay reported negative results but F1CDx reported positive for L858R with AF 33%. Upon further review, F1CDx identified a second somatic mutation in-cis (on same allele) as that of L858R with identical AF only 17bp downstream: *EGFR* A864P. Therefore, it is suspected that this second mutation interfered with the allele-specific PCR primers of **cobas**[®] EGFR v2, and thus L858R went undetected.

** QRF005867 was reported as positive for both replicates of **cobas**[®] EGFR v2 for exon19 deletion, but negative by F1CDx. F1CDx detected the exon19 deletion, but incorrectly annotated the variant as 2 frameshift mutations. This would have been corrected by manual curation review, which was not part of this concordance study. QRF005883 was also reported as positive for both replicates of **cobas**[®] EGFR v2 for exon19 deletion, but negative by F1CDx. F1CDx identified an 18bp exon 19 insertion event, with protein effect K745_E746insIPVAIK. As **cobas**[®] EGFR v2 is not designed to detect insertion events at exon 19, it is likely an error by **cobas**[®] EGFR v2.

Fifteen (15) samples were assigned as missing data for F1CDx, two of which also had missing results for CCD2. Missing data was caused by process failures or samples not meeting assay specifications.

By defining the reference standard as the consensus calls between CCD1 and CCD2, F1CDx achieved a PPA of 98.1% (106/108) (95% CI [93.5%, 99.8%]) and NPA of 99.4% (153/154) (95% CI [96.4%, 100.0%]). These data are summarized in Table 24.

Table 24. Summary of concordance data using agreement between CCD1 and CCD2 as the reference.

	CCD1+/CCD2+	CCD1-/CCD2-
F1CDX+	106	1
F1CDX-	2	153

The mutations detected by the **cobas**[®] EGFR v2 include all the mutations detected by *therascreen*[®] EGFR RGQ PCR Kit (QIAGEN), as well as a few additional exon19 deletions/L858R variants. Several concordance studies comparing the **cobas**[®] EGFR v2 and *therascreen*[®] EGFR RGQ PCR Kit have been reported in the literature^{2,3,4}, supporting that these two assays are concordant.

Additionally, a post-market concordance study will be completed comparing F1CDx to the *therascreen*[®] EGFR RGQ PCR Kit.

In addition, based on results of the FLAURA (NCT02296125) study, an additional therapeutic product, osimertinib, was approved on April 18, 2018, for the first-line treatment of patients with metastatic NSCLC whose tumors have EGFR exon 19 deletions or exon 21 L858R mutations, as detected by an FDA approved test. The companion diagnostic for this indication included the **cobas**[®] EGFR Mutation Test v2 (Roche Molecular Systems) whose claims were expanded, to include Tagrisso[®] (osimertinib) for the same *EGFR* exon 19 deletions and *EGFR* exon 21 L858R alterations as approved in the F1CDx PMA (P170019) on November 30, 2017. Consequently, Tagrisso[®] (osimertinib) was added to the F1CDx label for *EGFR* exon 19 deletions and *EGFR* exon 21 L858R alterations in NSCLC patients.

3.2 FoundationOne[®]CDx Concordance Study for *EGFR* T790M

The study established the clinical validity of the FoundationOne[®]CDx (F1CDx) as a companion diagnostic device used for identifying NSCLC patients harboring *EGFR* T790M that may be eligible for treatment with Tagrisso[®] (osimertinib). The patient samples and corresponding demographic information were obtained from AstraZeneca in connection with the clinical studies entitled AURA (NCT01802632), AURA2 (NCT02094261) and AURA3 (NCT02151981). The *EGFR* T790M diagnostic results from the F1CDx assay were compared against the consensus calls between the original T790M testing used in the AURA, AURA2 and AURA3 studies and a separate run of the FDA approved **cobas**[®] EGFR v2 (Roche Molecular Systems; designated as comparator companion diagnostic, CCD), using an NI approach.

Two separate concordance analyses were performed: one included samples with complete records only (N = 227), and the second analysis was with all the 312 samples, where missing data was handled by multiple imputation. A summary of concordance is presented in Table 25.

Table 25. Concordance table with CCD1, CCD2 and F1CDX results with eligible samples.

	CCD1+				CCD1-			
	CCD2+	CCD2-	CCD2 missing	Total	CCD2+	CCD2-	CCD2 missing	Total
F1CDx+	87	19	1	107	8	15	0	23
F1CDx-	1	4	0	5	0	93	2	95
F1CDx Missing	21	4	8	33	1	37	11	49
Total	109	27	9	145	9	145	13	167

Eighty-two samples were assigned as missing data for F1CDx, which consisted of 78 samples with no sequencing results from F1CDx and four samples with QC status as “Fail” after curation. CCD2 had 22 samples with missing data in total, in which 19 samples also had missing values in F1CDx.

The concordance analysis above shows that for the results of PPA, F1CDx is more concordant with both CCD1 and CCD2 than CCD1 is with CCD2; the opposite is true for NPA results. See the Venn Diagram below for the T790M-positive calls (Figure 2).

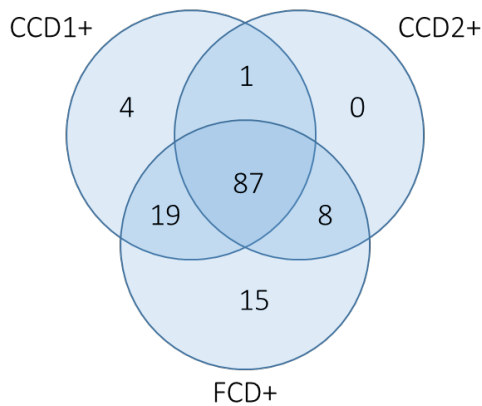


Figure 2. Venn Diagram for EGFR T790M-positive samples.

A difference in detection sensitivity between CCD1 and CCD2 was observed, with CCD1 appearing to be more sensitive than CCD2. This could be attributed to the fact that CCD1 was run 2-3 years ago using freshly biopsied tissue, while CCD2 testing was recently performed using DNA extracted from archival FFPE sections. Figure 3 below illustrates the relationship between allele frequency and detection by F1CDx, CCD1 and CCD2. The results demonstrated that F1CDx detects mutations at allele frequency lower than 5% which are not detected by the **cobas**® v2 assay. The clinical performance in this subset of the patient population (patients with an EGFR T790M mutation detected with an allele fraction <5%) is ongoing and has not been established.

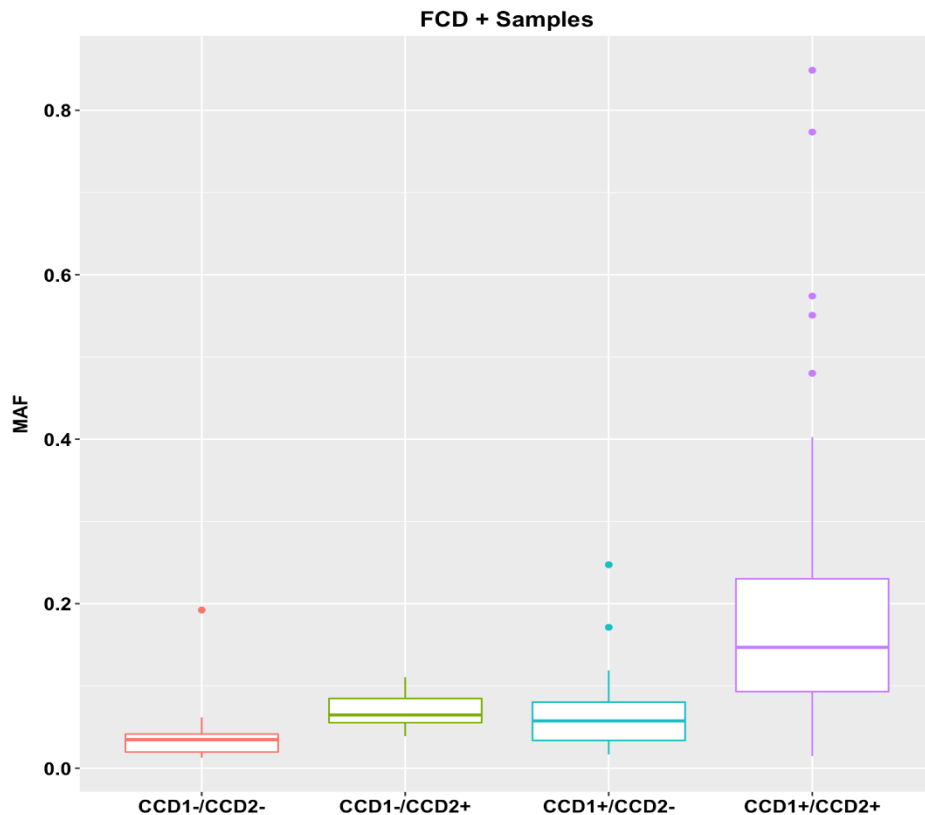


Figure 3. Distribution of MAF in F1CDx+ (FCD) samples.

By defining the reference standard as the consensus calls between CCD1 and CCD2, F1CDx achieved a PPA of 98.9% (87/88) (95% CI [93.8%, 100.0%]) and NPA of 86.1% (93/108) (95% CI [78.1%, 92.0%]) as summarized in Table 26 below.

Table 26. Summary of concordance data using agreement between CCD1 and CCD2 as the reference.

	CCD1+/CCD2+	CCD1-/CCD2-
F1CDx+	87	15
F1CDx-	1	93

3.3 FoundationOne®CDx Concordance Study for ERBB2 (HER2)

Clinical validity of FoundationOne®CDx (F1CDx) as a companion diagnostic device used to identify patients eligible for treatment with approved HER2-directed therapies including Herceptin® (trastuzumab), Kadcyła® (ado-trastuzumab-emtansine), and Perjeta® (pertuzumab) was established. A study was performed using 317 pre-screened retrospective samples obtained from patients with advanced breast cancer. The failure rate for pre-screening is not known; however, the sample set is enriched for samples with HER2+ samples with ratio between 2 and 3 representing 27% of samples compared to the expected range of 8-10% reported in literature^{5,6}. The ERBB2 amplification positive results from the F1CDx assay were compared against those obtained from the approved HER2 FISH PharmDx® Kit (Dako Denmark A/S). The samples used for this study were not obtained from a clinical trial and had limited demographic data available. For this study age and ethnicity data were available. Age data were compared to the Danish Study for the Danish Breast Cancer Group clinical trial 89-D in 1990 and was found to have a similar distribution, though the mean age was higher for the concordance samples.

Concordance data are summarized in Table 27 below.

Table 27. Concordance Table with CCD1, CCD2 and F1CDx results with eligible samples.

	CCD1+			CCD1-		
	CCD2+	CCD2-	Total	CCD2+	CCD2-	Total
F1CDx+	101	2	103	3	3	6
F1CDx-	12	10	22	6	180	186
Total	113	12	125	9	183	192

The prevalence of the *ERBB2*/HER2 amplification mutation in the intended use (IU) population is based on the ASCO guideline and is estimated to be 17.5%. To assess the impact of prevalence for the main results of this study, a sensitivity analysis was performed using the lower and upper bound of the prevalence guideline of 15% and 20%. The sensitivity analysis also showed that there was no impact on the study conclusion. The distribution of age is similar to the IU population for all samples tested. However, there was missing demographic data from the sample population. For missing data analysis using multiple imputation, the results show that based on the missing at random (MAR) assumption, the invalid test results did not affect the conclusion of this study.

The Venn diagrams for samples tested positive or negative for *ERBB2*/HER2-amplification mutation in all three assays (F1CDx, CCD1 and CCD2) are presented in Figure 4.

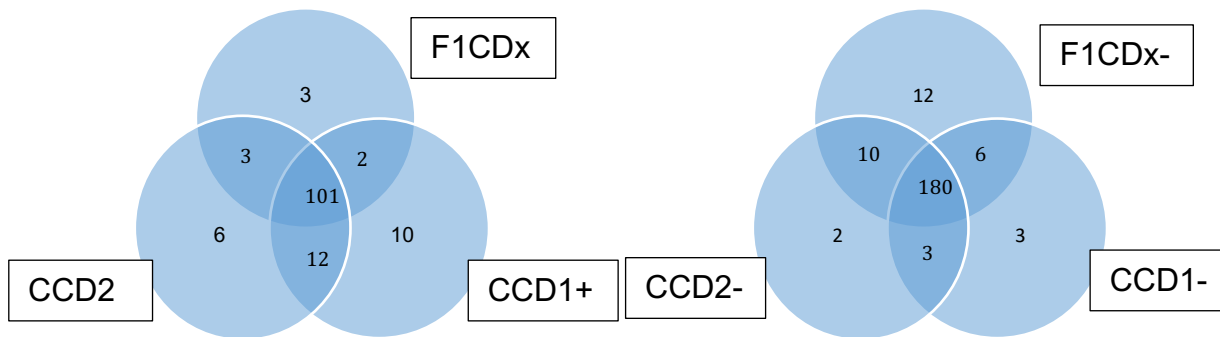


Figure 4. Venn Diagrams for *ERBB2*-amplification positive (left panel) and negative (right panel) samples.

These two Venn diagrams illustrate concordance among F1CDx, CCD1 and CCD2. For the F1CDx+ samples, concordance of F1CDx with CCD1 or CCD2 was better than concordance between the same platform tests CCD1 and CCD2; for the F1CDx- samples, F1CDx was more consistent in calling negative alterations than either CCD1 or CCD2.

Using the consensus calls between CCD1 and CCD2 as the reference standard, i.e., limiting analysis to only the samples in which CCD1 and CCD2 are in agreement, the results are shown below:

Table 28. Summary of concordance data using agreement between CCD1 and CCD2 as the reference.

	CCD1+/CCD2+	CCD1-/CCD2-
F1CDx+	101	3
F1CDx-	12	180

Based on these results, PPA is 89.4% (101/113) (95% CI [82.2%, 94.4%]) and NPA is 98.4% (180/183) (95% CI [95.3%, 99.7%]).

3.4 FoundationOne®CDx Concordance Study for ALK

Clinical validity of FoundationOne®CDx (F1CDx) as a companion diagnostic device used to identify non-small cell lung cancer (NSCLC) patients eligible for treatment with approved *ALK*-directed therapies including Alecensa® (alectinib), XALKori® (crizotinib), or Zykadia® (ceritinib) was established. The study was performed using 175 tumor samples from patients with histologically-confirmed NSCLC including enrolled patients as well as screen failures from the clinical trial NCT02075840, Roche study number BO28984 (also known as the ALEX study), which is a randomized, active controlled, multicenter Phase III open-label study designed to evaluate the efficacy and safety of alectinib compared with crizotinib treatment in participants with treatment-naïve *ALK* rearrangement positive advanced NSCLC. The *ALK* diagnostic results from the F1CDx panel were compared against those obtained from the FDA approved Ventana *ALK* (D5F3) CDx Assay (“Ventana IHC”, Ventana Medical Systems, Inc.) and Vysis *ALK* Break-Apart FISH Probe Kit (“Vysis FISH”, Abbott Molecular). The Vysis FISH assay results used were obtained from the ALEX study. In this concordance study, the majority of the samples were from the IU population of the clinical trial NCT02075840. The concordance results are summarized in Table 29 below.

Table 29. Concordance table with CCD1, CCD2 and F1CDx results with eligible samples.

	CCD1 +			CCD1 -		
	CCD2 +	CCD2 -	Total	CCD2 +	CCD2 -	Total
F1CDx +	78	1	79	3	0	3
F1CDx -	6*	7	13	5	75	80
Total	84	8	92	8	75	83

*Two samples harbored *ALK* rearrangements that were detected by F1CDx but were classified as negative based on the study protocol.

The Venn diagrams for samples tested positive or negative for *ALK*-rearrangement mutation in all three assays (F1CDx, CCD1 and CCD2) are shown in Figure 5.

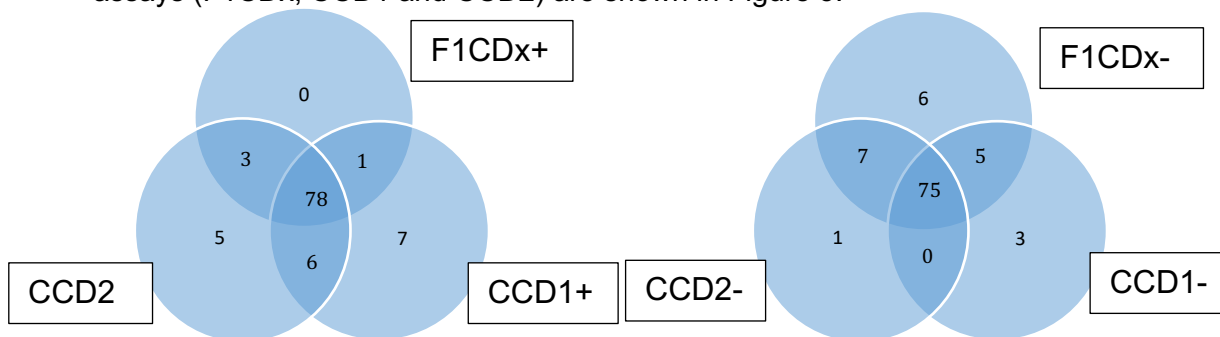


Figure 5. Venn Diagrams for *ALK*-rearrangement positive (left panel) and negative (right panel) samples.

These two Venn diagrams illustrate concordance among F1CDx, CCD1 and CCD2. A number of samples with discordant results between CCD1 and CCD2 were observed. This is expected because Vysis FISH Assay (CCD2) is a technology that probes at the DNA level while Ventana *ALK* IHC assay examines protein expression. When samples that were discordant between CCD1 and CCD2 were excluded, the concordance between F1CDx+ with CCD1+ and CCD2+ samples was superior to concordance between CCD1+ and CCD2+ samples. For the F1CDx- samples, F1CDx was more consistent in calling negative alterations than either CCD1 or CCD2.

Using the consensus calls between CCD1 and CCD2 as the reference standard, i.e. limiting analysis to only the samples in which CCD1 and CCD2 are in agreement, the results are shown below:

Table 30. Summary of concordance data using agreement between CCD1 and CCD2 as the reference.

	CCD1+/CCD2+	CCD1-/CCD2-
F1CDx+	78	0
F1CDx-	6*	75

*Two samples harbored *ALK* rearrangements that were detected by F1CDx but were classified as negative based on the study protocol.

Based on these results, PPA is 92.9% (78/84) (95% CI [85.1%, 97.3%]) and NPA is 100% (75/75) (95% CI [95.2%, 100.0%]).

3.5 FoundationOne®CDx Concordance Study for KRAS

Clinical validity of FoundationOne®CDx (F1CDx) as a companion diagnostic device used to identify colorectal cancer patients that may not benefit from certain *EGFR* inhibitor treatments, including Erbitux® (cetuximab) or Vectibix® (panitumumab), due to alterations in *KRAS* was established. The study was performed using 342 retrospective samples obtained from patients with advanced front-line or later-line colorectal cancer (CRC). Samples used in this study underwent pre-screening using the FoundationOne laboratory developed test (F1 LDT) or prescreening by an external vendor to enrich for positive samples. The prescreen failure rate using the F1 LDT was 3.7% and is unknown for the external vendor. The *KRAS* diagnostic results from the F1CDx assay were compared against those obtained from the approved *therascreen*® *KRAS* RGQ PCR Kit (QIAGEN). The samples used for this study were not obtained from a clinical trial and had limited demographic data available. For this study age, gender and ethnicity data were available. Age and gender characteristics were found to be similar between the F1CDx concordance study and the pivotal studies, with the percentage of male samples in the concordance study being slightly lower compared to the pivotal studies (CRYSTAL and PRIME). Concordance data are summarized in Table 31 below.

Table 31. Concordance Table with CCD1, CCD2 and F1CDx results with eligible samples.

	CCD1+				CCD1-			
	CCD2+	CCD2-	CCD2 missing	Total	CCD2+	CCD2-	CCD2 missing	Total
F1CDx+	173	0	2	175	0	0	0	0
F1CDx-	0	2	0	2	1	154	7	162
F1CDx Missing	0	0	0	0	0	3	0	3
Total	173	2	2	177	1	157	7	165

Twelve (12) samples are assigned as missing data, including 3 samples with missing data in F1CDx and 9 samples with missing data in CCD2.

The prevalence of the *KRAS* mutation in the IU population is based on the CRYSTAL study for cetuximab (35.6%) and PRIME study for panitumumab (40%). The key statistics of PPA and NPA between F1CDx and the two replicates of the *therascreen*® *KRAS* assay (CCD1 and CCD2) were estimated based on the result in Table 32. Multiple imputation was used to impute the missing data and showed that missing data did not impact study conclusions. The summary statistics of age and sex were highly similar to the estimates from the pivotal trial CRYSTAL (for cetuximab) and PRIME (for panitumumab) studies.

By defining the reference standard as the consensus calls between CCD1 and CCD2, F1CDx achieved a PPA of 100% (173/173) (95% CI [97.9%, 100.0%]) and NPA of 100% (154/154) (95% CI [97.6%, 100.0%]).

Table 32. Summary of concordance data using agreement between CCD1 and CCD2 as the reference.

	CCD1+/CCD2+	CCD1-/CCD2-
F1CDx+	173	0
F1CDx-	0	154

3.6 FoundationOne®CDx Concordance Study for BRAF

Clinical validity of the FoundationOne®CDx (F1CDx) as a companion diagnostic device used to identify melanoma patients that may be eligible for treatment with approved BRAF-directed therapies was established. The study was performed using 305 retrospective samples obtained from patients with advanced melanoma. 157 samples used in this study underwent pre-screening using the FoundationOne laboratory developed test (F1 LDT) and 27 were prescreened by an external vendor to enrich for positive samples. The prescreen failure rate using the F1 LDT was 3.7% and is unknown for the external vendor. The BRAF diagnostic results from the F1CDx assay were compared against those obtained from the approved cobas® 4800 BRAF V600 Mutation Test (Roche Molecular Systems, Inc; referred to as the cobas® BRAF assay below). These samples were not obtained from a clinical trial and had demographic data limited to age and gender. The distributions of age and gender to the intended use population (BRIM-3 trial) was found to be comparable.

Concordance analysis showed that the upper bounds of 95% one-sided Confidence Interval (CI) were below 20% for all four NI hypothesis tests. Thus, it can be concluded with 95% confidence that the differences of results between F1CDx and cobas® BRAF assays are less than 20%, the non-inferiority (NI) margin. Concordance results are summarized in Table 33 below.

Table 33. Concordance Table with CCD1, CCD2 and F1CDx results with eligible samples.

	CCD1+			CCD1-		
	CCD2+	CCD2-	Total	CCD2+	CCD2-	Total
F1CDx+	166	0	166	3	14	17
F1CDx-	1	0	1	0	121	121
Total	167	0	167	3	135	138

Because the cobas® BRAF assay has lower sensitivity for detection of dinucleotide mutations, a separate analysis was conducted that included only eligible samples without dinucleotide mutations. A total of 273 (=305-32) samples were available for this analysis. The concordance results are summarized in Table 34.

Table 34. Concordance Table with CCD1, CCD2 and F1CDx results with eligible samples excluding samples with dinucleotide mutations detected by F1CDx.

	CCD1+			CCD1-		
	CCD2+	CCD2-	Total	CCD2+	CCD2-	Total
F1CDx+	149	0	149	1	1*	2
F1CDx-	1**	0	1	0	121	121
Total	150	0	150	1	122	123

*QRF006472 was the only sample where both replicates of the cobas® BRAF assay reported negative results but F1CDx reported positive. The Allele Frequency of this sample was 3.45% with the computational tumor purity of 10%. According to Table 4 of the cobas® BRAF assay insert, the cobas® BRAF assay can correctly detect all BRAF V600E mutant specimens that have a minimum % mutant DNA above 5% and when the minimum tumor content is at least 15%. Thus, the discordance can be explained by F1CDx's high sensitivity in the lower % mutant DNA and low tumor purity condition.

**QRF006374 was the only sample where both replicates of the cobas® BRAF assay reported positive results but F1CDx reported negative. A mutation was recorded in the line data (Appendix 7) having protein effect V600_K601>E, which is a non-frameshift deletion of 3 nucleotides with CDS effect 1799_1801delTGA. This more

complex mutation does result in V600E, but because of annotation differences to the canonical V600E, it was called negative by F1CDx.

PPA and NPA were calculated by defining the reference standard as the consensus calls between CCD1 and CCD2. The observed performance of **cobas**[®] BRAF assay has lower sensitivity for detection of dinucleotide V600 alterations (including V600K) than the single nucleotide V600E 1799T>A alteration, particularly at allele frequency below 40% detected by F1CDx, therefore, the data presented will include PPA/NPA results both with both alterations as the study was designed, as well as for V600E only in Table 35. A study using the THxID[™] BRAF kit (bioMérieux) was conducted using 29 samples with BRAF V600 dinucleotide mutation detected by F1CDx and 29 negative samples to provide a better evaluation of V600 dinucleotide concordance. Out of the 51 samples with valid results from the THxID[™] BRAF kit (Table 36), there was only one discordant result (F1CDx-/THxID+), achieving a PPA of 96.3% (26/27) (95% CI [81.0%, 99.9%]) and NPA of 100% (24/24) (95% CI [85.8%, 100.0%]).

Table 35. PPA and NPA for BRAF V600 detection with cobas[®] BRAF.

	PPA	NPA
All V600 alterations	99.4% (166/167)	89.6% (121/135)
Single nucleotide V600E (1799T>A)	99.3% (149/150)	99.2% (121/122)

Table 36. Concordance of BRAF dinucleotide samples with THxID[™] BRAF kit.

Dinucleotide Samples	THxID+	THxID-	Total
F1CDx+	26	0	26
F1CDx-	1	24	25
Total	27	24	51

3.7 Summary of Clinical Concordance Studies

A summary of clinical concordance study results is included in Table 37 below. The reference standard used to calculate positive percent agreement (PPA) and negative percent agreement (NPA) below is defined as the consensus calls between the two comparator methods or comparator runs. Agreement calculations solely using consensus calls may overestimate the performance of FoundationOne[®]CDx (F1CDx).

Table 37. Summary of PPA and NPA for CDx concordance studies.

Biomarker	PPA	NPA	Comparator Method
EGFR exon 19 deletions and L858R	98.1% (106/108)	99.4% (153/154)	cobas [®] EGFR Mutation Test v2
EGFR T790M	98.9% (87/88)	86.1% (93/108)	cobas [®] EGFR Mutation Test v1 cobas [®] EGFR Mutation Test v2
ALK rearrangements	92.9% (78/84)	100% (75/75)	Ventana ALK (D5F3) CDx Assay Vysis ALK Break-Apart FISH Probe Kit
KRAS	100% (173/173)	100% (154/154)	<i>therascreen</i> [®] KRAS RGQ PCR Kit
ERBB2(HER2) Amplifications	89.4% (101/113)	98.4% (180/183)	Dako HER2 FISH PharmDx [®] Kit
BRAF V600	99.4% (166/167)	89.6% (121/135) ¹	cobas [®] 4800 BRAF V600 Mutation Test
BRAF V600E	99.3% (149/150)	99.2% (121/122)	cobas [®] 4800 BRAF V600 Mutation Test
BRAF V600 dinucleotide ²	96.3% (26/27)	100% (24/24)	THxID [™] BRAF kit

¹ Sensitivity of dinucleotide detection of *BRAF* V600K and V600E was found to be significantly reduced in **cobas**[®] *BRAF* test, in particular for samples in which F1CDx detected the dinucleotides to be of lower than 40% MAF, leading to low NPA values.

² A study using the THxIDTM *BRAF* kit (bioMérieux) was conducted with samples with *BRAF* V600 dinucleotide mutation detected by F1CDx and *BRAF* V600 negative samples to provide a better evaluation of V600 dinucleotide concordance.

3.8 FoundationOne[®]CDx Concordance with FoundationFocus CDx_{BRCA LOH} for *BRCA1*, *BRCA2*, and LOH calling

FoundationOne[®]CDx (F1CDx) and FoundationFocus CDx_{BRCA LOH} assays are equivalent with the exception of an updated analysis pipeline in use for F1CDx and reporting software that allow for comprehensive reporting of all relevant alterations detected by the F1CDx platform. Comprehensive validation of the analysis pipeline which included robust regression testing and reanalysis of FoundationFocus CDx_{BRCA LOH} clinical bridging sample data was performed. The assays were determined to be concordant for determining HRD status. Reanalysis of the clinical efficacy data demonstrated that F1CDx and FFocus have similar performance in identifying HRD+ patients who may benefit from rucaparib treatment. Details for the clinical studies can be found in the Summary of Safety and Effectiveness Data for PMA P160018 and P160018/S001. A summary of progression-free survival assessed by the investigator using F1CDx is provided in Table 38 below.

Table 38. Progression-free survival assessed by the investigator (invPFS) using F1CDx.

Cohort	Hazard Ratio Rucaparib vs Placebo	Number of Patients	Median invPFS (months)		95% CI
ITT	0.365	375	10.8	Rucaparib	8.3, 11.4
	P value: <.0001				
	95% CI: 0.295, 0.451	189	5.4	Placebo	5.3, 5.5
All populations assessable by FMI assays	0.377	345	10.4	Rucaparib	8.3, 11.1
	P value: <.0001				
	95% CI: 0.302, 0.469	173	5.4	Placebo	5.3, 5.5
HRD+	0.302	215	13.6	Rucaparib	10.9, 17.1
	P value: <.0001				
	95% CI: 0.224, 0.406	110	5.4	Placebo	5.1, 5.6
tBRCA+	0.240	124	16.6	Rucaparib	11.1, 22.9
	P value: <.0001				
	95% CI: 0.159, 0.364	63	5.4	Placebo	4.9, 7.1
tBRCA- LOH+	0.354	91	9.7	Rucaparib	8.2, 13.8
	P value: <.0001				
	95% CI: 0.226, 0.554	47	5.4	Placebo	2.9, 5.6
tBRCA- LOH unknown	0.176	16	8.3	Rucaparib	5.3, 24.7
	P value=0.0069				
	95% CI: 0.044, 0.711	8	4.1	Placebo	2.3, 8.2
tBRCA- LOH-	0.620	114	6.3	Rucaparib	5.4, 8.3
	P value=0.0086				
	95% CI: 0.429, 0.895	55	5.4	Placebo	4.1, 5.6

3.9 Clinical evaluation of *BRCA1/2* classification for treating ovarian cancer patients with olaparib

3.9.1 Summary of the Clinical Study – Olaparib D0818C00001 (SOLO1)

The clinical performance of F1CDx for *BRCA1/2* classification was established based on available tumor analysis using the F1CDx in the clinical study D0818C00001 (SOLO1). SOLO1 was a Phase III, randomized, double-blind, placebo-controlled, multicenter trial, that compared the efficacy of Lynparza[®] (olaparib) with placebo in patients with advanced ovarian, fallopian tube, or primary peritoneal cancer with *BRCA* mutation (documented mutation in *BRCA1* or *BRCA2*) following first-line platinum-based

chemotherapy. A total of 391 patients were randomized (2:1) to receive Lynparza tablets 300 mg orally twice daily (n=260) or placebo (n=131). Patients were required to have a documented mutation in *BRCA1* or *BRCA2* that were known or predicted to be a loss of function mutation.

Treatment was continued for up to 2 years or until disease progression or unacceptable toxicity; however, patients with evidence of disease at 2 years, who in the opinion of the treating healthcare provider could derive further benefit from continuous treatment, could be treated beyond 2 years. Randomization was stratified by response to first-line platinum-based chemotherapy (complete or partial response). The major efficacy outcome was investigator-assessed progression-free survival (PFS) evaluated according to Response Evaluation Criteria in Solid Tumors (RECIST), version 1.1.

The study was designed to recruit *BRCAm* patients, i.e., germline or somatic *BRCAm* (*gBRCAm* or *sBRCAm*). At the time of study initiation, a health authority approved tumor diagnostic test was not available. Patients known to have *BRCA* mutation/s (*gBRCA*, i.e., blood or *tBRCA*, i.e., tumor) prior to randomization could enter the study based on this result provided that all such testing had been undertaken in appropriately accredited laboratories (i.e., testing done for research use only [RUO] was not acceptable). In addition, the patients must have consented to provide blood samples for a confirmatory *gBRCA* test post randomization using a blood-based germline *BRCA* test. However, patients could enter the study if they were known to have a tumor *BRCAm* (*tBRCAm*) based on a local, clinically validated test. Tumor tissue was requested for all randomized patients and where possible, retrospectively tested prior to database lock with the F1CDx assay. Since few patients underwent tumor testing during the SOLO1 recruitment period, the patients recruited were predominantly *gBRCAm* as determined by local results or a *gBRCA* clinical trial assay (CTA); however, there were 2 patients with *sBRCAm* tumors. Based on strong biological rationale, it is predicted that patients with a *BRCA* mutation that is somatic in origin will derive a similar clinical efficacy benefit to those with a mutation that is germline in origin.

3.9.2 Accountability of the PMA Cohort

Out of the 391 patients randomized in SOLO1, 368 (94.1%) had an available tumor sample for testing. Of these, 335 (85.6%) patients had a valid tumor tissue F1CDx result. Out of the 335 with a valid tumor tissue F1CDx result, 313 patients were confirmed to carry a deleterious mutation in either *BRCA1* or *BRCA2* by F1CDx. The PMA cohort represented 80.1% of the full analysis set (FAS) in SOLO1. Of the 22 patients that were not confirmed to carry a deleterious mutation by F1CDx, 12 were not confirmed to have a deleterious mutation by F1CDx in their tumor tissue due to differences in the variant classification criteria used by F1CDx compared to the *gBRCA* CTA. The remaining 10 patients that were not confirmed to carry deleterious *BRCA1/2* mutations in their tumor tissue had genomic rearrangements that consisted of large-scale genomic deletions (affecting at least one whole exon), or large-scale genomic insertions including exon duplications. These patients represented 10 out of a total of 20 randomized patients in SOLO1 that had genomic rearrangements in *BRCA1/2* detected by the *gBRCA* CTA.

3.9.3 Efficacy Evaluation

The primary efficacy endpoint was investigator assessed PFS evaluated according to RECIST, version 1.1. SOLO1 met the primary endpoint demonstrating a statistically significant improvement in investigator-assessed PFS for olaparib compared to placebo. Results from a blinded independent review were consistent.

The effectiveness of the F1CDx test was based on a subset of 313 ovarian cancer patients whose tumor tissue was confirmed to carry deleterious *tBRCAm* status. Table 39 presents a summary of key efficacy outcome variables for patients whose tissue was confirmed to have *tBRCAm* status by F1CDx. PFS in the confirmed F1CDx *tBRCAm* patients was consistent with the results of the FAS, namely that SOLO1 met the primary endpoint, demonstrating a substantial improvement in PFS for olaparib compared with placebo. The sensitivity analysis of PFS to assess possible ascertainment bias using blinded independent centralized review (BICR) in the F1CDx confirmed *tBRCAm* patient subset was consistent with the BICR-assessed PFS analysis in the FAS and confirmed its robustness. Overall, the primary efficacy outcome in the F1CDx *tBRCAm* subset were consistent with the FAS.

Table 39. Summary of key efficacy outcome variables in the FAS and in the F1CDx *tBRCAm* subset.

	FAS n=391		F1CDx <i>tBRCAm</i> n=313	
	Olaparib (n=260)	Placebo (n=131)	Olaparib (n=206)	Placebo (n=107)
PFS by Investigator Assessment				
Number of events/total number of patients (%)	102/260 (39)	96/131 (73)	80/206 (39)	81/107 (76)
Median PFS (months) ^a	Not reached	13.8	Not reached	11.9
HR (95% CI) ^b	0.30 (0.23-0.41)		0.28 (0.20-0.38)	
p-value (2-sided) ^c	p<0.0001		p<0.0001	

^a PFS is defined as the time from randomization until data of RECIST progression or death.

^b Hazard ratio from a Cox proportional hazards model including response to previous platinum chemotherapy (complete response versus partial response) as a covariate.

^c The p-value is derived from a stratified log-rank test.

3.10 FoundationOne[®]CDx Clinical Bridging Study for *PIK3CA*

The safety and effectiveness of FoundationOne[®]CDx (F1CDx) for detecting *PIK3CA* alterations in breast cancer patients who may benefit from treatment with alpelisib was demonstrated in a retrospective analysis of specimens from patients enrolled in SOLAR-1. SOLAR-1 is the pivotal Phase III, randomized, double-blind, placebo controlled study of alpelisib in combination with fulvestrant in men and postmenopausal women with hormone receptor positive (HR+), human epidermal growth factor receptor 2 negative (HER2-) locally advanced breast cancer whose disease had progressed or recurred on or after an aromatase inhibitor based treatment (with or without CDK4/6 combination) (SOLAR-1, NCT2437318).

A bridging study was conducted to assess the clinical efficacy of F1CDx in identifying *PIK3CA* alteration positive patients for treatment with alpelisib in combination with fulvestrant and the concordance between *PIK3CA* status (mutant or non-mutant) tested with the clinical trial enrollment assays (referred to as clinical trial assay [CTA1] and [CTA2]) and the F1CDx in the intent-to-test population. F1CDx was used to retrospectively test the stored patient samples from SOLAR-1 with sufficient residual tumor material (N = 415 of the total 572 enrolled patients). Samples from 296 patients enrolled with the CTA1 (119 *PIK3CA* alteration positive patients and 177 *PIK3CA* alteration negative patients), and 119 patients enrolled with the CTA2 (115 *PIK3CA* alteration positive patients and 4 *PIK3CA* alteration negative patients), were retrospectively tested with F1CDx.

3.10.1 Safety Analysis

The F1CDx assay is not expected to directly cause actual or potential adverse effects, but test results may directly impact patient treatment risks.

3.10.2 Effectiveness Results

Concordance Analysis

The concordance between F1CDx and the two enrollment assays (CTA1 and CTA2) was assessed. The point estimates of PPA, NPA and OPA for F1CDx compared to the CTAs are provided in Table 40 and Table 41 below.

Table 40. Agreement between CDx and CTA1 based on the CTA1 results (Primary analysis set, CTA1-enrolled).

Measure of agreement	Without invalid CDx results		With invalid CDx results	
	Percent agreement (N)	95% CI (1)	Percent agreement (N)	95% CI (1)
PPA	93.8% (106/113)	(87.7%, 97.5%)	93.0% (106/114)	(86.6%, 96.9%)
NPA	98.8% (159/161)	(95.6%, 99.8%)	95.8% (159/166)	(91.5%, 98.3%)
OPA	96.7% (265/274)	(93.9%, 98.5%)	94.6% (265/280)	(91.3%, 97.0%)

(1) The 95% CI calculated using the Clopper-Pearson Exact method.

- Samples not tested are excluded from the analysis.

- Samples tested on deviation are excluded from the analysis.

Table 41. Agreement between CDx and CTA2 based on the CTA2 results (Concordance analysis set for CTA2).

Measure of Agreement	Without invalid CDx results		With invalid CDx results	
	Percent Agreement (N)	95% CI (1)	Percent Agreement (N)	95% CI (1)
PPA	91.6% (197/215)	(87.1%, 95.0%)	90.4% (197/218)	(85.7%, 93.9%)
NPA	98.8% (162/164)	(95.7%, 99.9%)	97.0% (162/167)	(93.2%, 99.0%)
OPA	94.7% (359/379)	(92.0%, 96.7%)	93.2% (359/385)	(90.3%, 95.5%)


(1) The 95% CI calculated using the Clopper-Pearson Exact method.

- Samples not tested are excluded from the analysis.

- Samples tested on deviation are excluded from the analysis.

Clinical Efficacy Results in the SOLAR-1 Mutant Cohort

The SOLAR-1 clinical trial met its primary objective demonstrating a statistically significant improvement in PFS by investigator assessment in patients with *PIK3CA* alteration positive tumors. Supportive analysis included PFS based on blinded independent review committee (BIRC). Alpelisib in combination with fulvestrant demonstrated an estimated 35% risk reduction of disease progression or death compared to the placebo plus fulvestrant arm (HR = 0.65; 95% CI: 0.50, 0.85; p = 0.00065) in the *PIK3CA* alteration cohort. The median PFS was prolonged by a clinically relevant 5.3 months, from 5.7 months in the placebo plus fulvestrant arm to 11.0 months in the alpelisib plus fulvestrant arm (Figure 6).

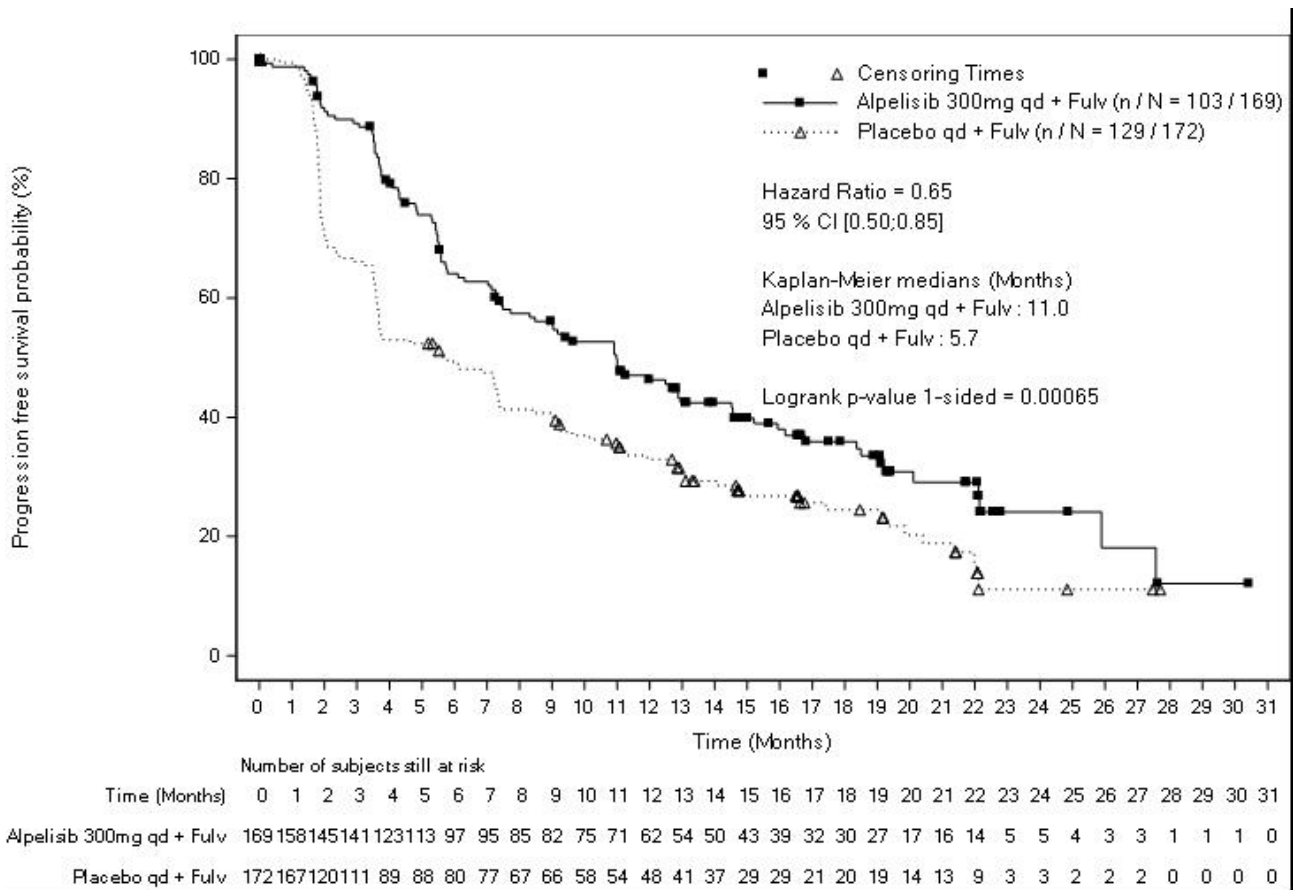

Stratified Logrank test and stratified Cox model using strata defined by (i) prior CDK 4/6 inhibitor use. (ii) presence of liver and/or lung metastases.

Figure 6. Kaplan-Meier plot of progression free survival by treatment in the mutant patients randomized in the original SOLAR-1 trial (Primary analysis set).

Clinical Efficacy Results in the CDx-Positive Population

Efficacy analyses were performed for patients determined to be CDx-positive (*PIK3CA* alteration detected by F1CDx) and compared to the efficacy results in the SOLAR-1 *PIK3CA* mutant cohort. The clinical efficacy in the CDx-positive population was estimated by pooling the hazard ratios calculated for 1) the CTA1-enrolled patients that were CDx-positive and 2) the CTA2-enrolled patients that were CDx-positive.

Table 42 and Table 43 show the efficacy results in the CTA1-enrolled CDx-positive patients (HR = 0.52, 95% CI: 0.29, 0.93) and the results in the CTA2-enrolled (CTA2+, CDx+) patients (HR = 0.35, 95% CI: 0.16, 0.77), respectively.

For the sensitivity analysis to c for the clinical efficacy of alpelisib in combination with fulvestrant for the *PIK3CA* CDx-positive population, the hazard ratio estimates ranged from 0.43 to 0.44. The upper bounds of the 95% confidence intervals for the corresponding hazard ratios were all below 1.0. Sensitivity analysis against the missing CDx results demonstrated the robustness of the efficacy analysis.

Table 42. Clinical efficacy on progression free survival in the CTA1-enrolled CDx-positive patients (Primary analysis set, CTA1-enrolled).

Progression free survival (months)	Alpelisib 300mg qd +		HR(95% CI) Alpelisib 300mg qd + Fulv / Placebo qd + Fulv (1)
	Fulv N=56	Placebo qd + Fulv N=52	
No of events (%)	41 (73.2)	41 (78.8)	0.52 (0.29, 0.93)
PD (%)	39 (69.6)	41 (78.8)	
Death (%)	2 (3.6)	0	
No of censored (%)	15 (26.8)	11 (21.2)	
Median (95% CI) (2)	11.2 (8.3, 18.5)	5.5 (1.9, 10.9)	

(1) Hazard ratio (HR) estimated using Cox regression model. The model is adjusted by the identified baseline clinical covariates, as well as the covariates that are imbalanced between treatment and control. The model is stratified by the two stratification factors: presence of lung and/or liver metastases, previous treatment with any CDK4/6 inhibitor.

CI: Wald Confidence Interval.

(2) The 95% CI calculated from PROC LIFETEST output using the method of Brookmeyer and Crowley (1982).

-CDx results obtained on deviation are treated as missing.

Table 43. Clinical efficacy on progression free survival in the CTA2-enrolled (CTA2+, CDx+) patients (Primary analysis set, CTA2-enrolled).

Progression free survival (months)	Alpelisib 300mg qd +		HR(95% CI) Alpelisib 300mg qd + Fulv / Placebo qd + Fulv (1)
	Fulv N=42	Placebo qd + Fulv N=48	
No of events (%)	19 (45.2)	36 (75.0)	0.35 (0.16, 0.77)
PD (%)	18 (42.9)	31 (64.6)	
Death (%)	1 (2.4)	5 (10.4)	
No of censored (%)	23 (54.8)	12 (25.0)	
Median (95% CI) (2)	10.9 (5.6, NE)	4.2 (2.1, 7.4)	

(1) Hazard ratio (HR) estimated using Cox regression model. The model is adjusted by the identified baseline clinical covariates, as well as the covariates that are imbalanced between treatment and control. The model is stratified by the two stratification factors: presence of lung and/or liver metastases, previous treatment with any CDK4/6 inhibitor.

CI: Wald Confidence Interval.

(2) The 95% CI calculated from PROC LIFETEST output using the method of Brookmeyer and Crowley (1982).

-CDx results obtained on deviation are treated as missing.

Conclusions

The data from this study support reasonable assurance of the safety and effectiveness of the F1CDx assay when used to aid clinicians in identifying breast cancer patients with *PIK3CA* alterations who may be eligible for treatment with alpelisib.

3.11 Clinical evaluation of *FGFR2* rearrangement detection for treating Cholangiocarcinoma (CCA) patients with pemigatinib

The clinical performance of F1CDx for detecting *FGFR2* fusions and rearrangements in CCA patients who may benefit from treatment with pemigatinib was established with clinical data generated from the Incyte trial INCB 54828-202, and a clinical bridging study to establish concordance between the confirmatory clinical trial assay (CTA) and the F1CDx assay.

3.11.1 Summary of the Clinical Study – INCB 54828-202 (FIGHT-202)

Study INCB 54828-202 is a prospective, multicenter, open-label, Phase II study in participants with previously treated, advanced/metastatic or surgically unresectable cholangiocarcinoma, including participants with *FGFR2*-rearranged cholangiocarcinoma. The primary endpoint of Study INCB 54828-

202 was the objective response rate (ORR) in participants with *FGFR2*-rearranged cholangiocarcinoma to determine whether treatment with pemigatinib is safe and effective. Participants in Study INCB 54828-202 were assigned to cohorts for statistical analysis based on tumor *FGF/FGFR* status as determined by the FMI F1 CTA: Cohort A included participants with *FGFR2* fusions and select rearrangements in cholangiocarcinoma, and Cohorts B and C included participants with other cholangiocarcinoma molecular subtypes. Eligible participants received pemigatinib on a 2-weeks-on/1-week-off schedule at a starting dose of 13.5 mg once a day. Treatment continued until documented disease progression or unacceptable toxicity.

In the trial, *FGFR2* candidate fusions and rearrangements were defined as the following:

- An *FGFR2* rearrangement predicted to be a fusion: Breakpoint is within the *FGFR2* intron 17/exon 18 hotspot and the gene partner is known in the literature, in strand with *FGFR2*; or is a novel partner that is predicted to be in strand and in frame with *FGFR2*.
- An *FGFR2* rearrangement, which cannot be conclusively predicted to be a fusion: Breakpoint is within the *FGFR2* intron 17/exon 18 hotspot but the partner gene is out of frame or out of strand with exon 17 of *FGFR2*. Alternatively, the downstream end of the breakpoint may be in an intergenic region and not within another gene (designated as partner n/a).

3.11.2 Accountability of the PMA Cohorts

A total of 146 participants with previously treated, advanced/metastatic or surgically-unresectable cholangiocarcinoma were enrolled in Study INCB 54828-202. Based on tumor sample testing from the FMI F1 CTA, 145 participants were included in the efficacy evaluable population after one participant was not able to be confirmed by the F1 CTA. The 145 participants were assigned to one of the following cohorts for statistical analyses:

- Cohort A: 107 participants with *FGFR2* fusions/rearranged cholangiocarcinoma
- Cohort B: 20 participants with other *FGF/FGFR* alterations
- Cohort C: 18 participants with tumors negative for *FGF/FGFR* alterations

The efficacy of PEMAZYRE was determined in cohort A (107) patients with locally advanced unresectable or metastatic cholangiocarcinoma whose disease had progressed on or after at least 1 prior therapy and who had an *FGFR2* gene fusion or non-fusion rearrangement, as determined by the clinical trial assay. Qualifying in-frame fusions and other rearrangements were predicted to have a breakpoint within intron 17/exon 18 of the *FGFR2* gene leaving the *FGFR2* kinase domain intact.

3.11.3 Efficacy Evaluation

3.11.3.1 Clinical efficacy results in Intent to Treat population

The major efficacy outcome measures were overall response rate (ORR) and duration of response (DoR) as determined by an independent review committee (IRC) according to RECIST v1.1. The results of this study are shown in Table 44 below.

Table 44. Efficacy results in FIGHT-202 trial.

Efficacy Parameter	PEMAZYRE N = 107
ORR (95% CI)	36% (27, 45)
Complete response	2.8%
Partial response	33%

3.11.3.2 Summary of the Clinical Bridging Study

Following testing by the F1 CTA, residual DNA for patients in INCB 54828-202 was banked to support the clinical bridging study testing with the F1CDx assay. The safety and effectiveness of F1CDx for detecting *FGFR2* rearrangements in CCA patients who may benefit from treatment with pemigatinib was demonstrated in a retrospective analysis of residual DNA from patients enrolled in the INCB 54828-202

trial. Residual DNA was available for 108 patients screened with the CTA (80 in Cohort A, 14 in Cohort B, 10 in Cohort C, and 4 screen failures). In addition to 73 *FGFR2* rearrangement-negative specimens for a total of 181 positive and negative F1CDx evaluable samples included in the analysis. A bridging study was conducted to assess the clinical efficacy of F1CDx in identifying *FGFR2* rearrangement positive patients for treatment with pemigatinib and the concordance between *FGFR2* rearrangement status (mutant and non-mutant) tested with the CTA and F1CDx in the efficacy evaluable population. Of the evaluable specimens in cohort A (n=80), the most common finding was *FGFR2-BICC1* [27% (22/80)] in the evaluable set. Patients also had rearrangements without an identifiable partner gene. All of the biomarker positive cases in the F1CDx *FGFR2* CCA Clinical Bridging Study had breakpoints in the *FGFR2* hotspot region, intron 17 – exon 18. (Figure 1)

Clinical efficacy results in the CDx-positive population

Clinical utility of F1CDx was evaluated by estimation of clinical efficacy in the *FGFR2* rearranged, CTA-enrolled population based on the primary objective of ORR per central review per RECIST v1.1 criteria. Sensitivity analysis, using the multiple imputation method, was performed to evaluate the robustness of the clinical efficacy estimate against the 27 missing CDx results from Cohort A and 14 missing results from cohort B and C combined. The ORR for the F1CDx *FGFR2*-rearrangement-positive population estimated by the bridging study was 37.50% and aligns with the ORR for the CTA *FGFR2*-rearrangement-positive population, which was 35.51% (Table 45). Sensitivity analysis, using the multiple imputation method, was performed to evaluate the robustness of the clinical efficacy estimate against the 27 missing CDx results from the efficacy evaluable population (Cohort A). The distribution of *FGFR2* fusions in the trial that were available for bridging is shown in Figure 7 below.

Table 45. Summary of ORR in different subpopulations for completed data.

Population	CTA+	CTA+ and F1CDx+	CTA+ and F1CDx-
n	107	80	0
ORR	35.51%	37.50%	N/A
95% 2-sided exact CIs	[26.50%,45.35%]	[26.92%,49.04%]	N/A

Note: Given the NPA=1, the efficacy of F1CDx *FGFR2* rearrangement positives can be estimated from the (CTA+, F1CDx+) group.

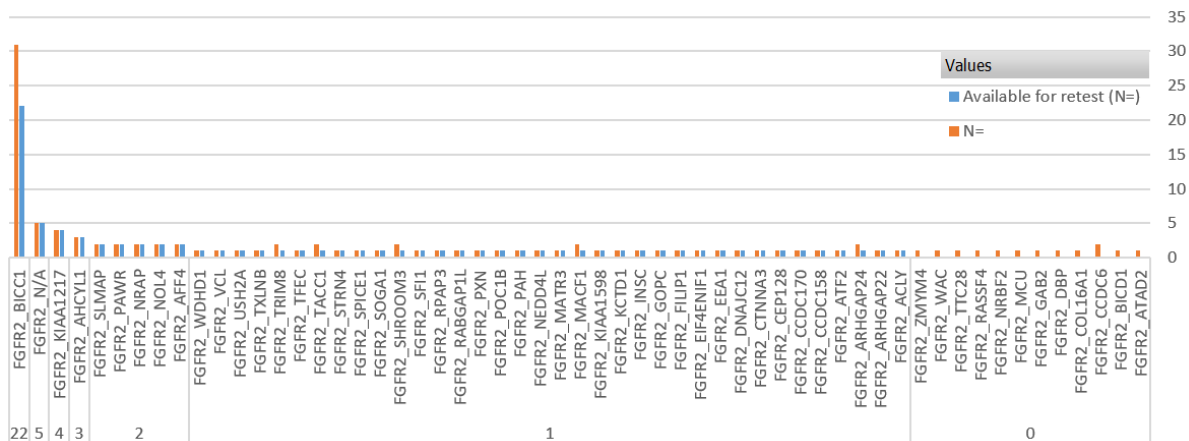


Figure 7. Distribution of FGFR2 fusions and rearrangements in Cohort A in support of efficacy.

3.11.3.3 Safety Analysis

The F1CDx assay is not expected to directly cause actual or potential adverse effects, but test results may directly impact patient treatment risks.

3.11.3.4 Clinical Concordance

Patients with valid F1CDx results together with FMI archived samples were used to demonstrate concordance of F1CDx to the CTA. Retrospective testing with F1CDx yielded 181 CDx-evaluable results used for further analysis (84 positive and 97 negative). Agreement between F1CDx and the CTA was demonstrated. The PPA, NPA, OPA, adjusted PPV, and adjusted NPV all exhibited 100% agreement between the F1CDx assay and the F1 CTA.

3.11.3.5 Conclusions

The data from this study support reasonable assurance of the safety and effectiveness of the F1CDx assay when used to aid clinicians in identifying CCA patients with *FGFR2* fusions and rearrangements who may be eligible for treatment with pemigatinib.

3.12 Clinical evaluation of *MET* exon 14 classification for treating NSCLC patients with capmatinib

The clinical performance of F1CDx for detecting SNVs and indels that lead to *MET* exon 14 skipping in NSCLC patients who may benefit from treatment with capmatinib was established with clinical data generated from the Novartis trial CINC280A2201 (GEOMETRY-mono 1), and a clinical bridging study to establish concordance between the enrollment clinical trial assay (CTA) and the F1CDx assay.

3.12.1 Summary of the Clinical Study – CINC280A2201 (GEOMETRY-mono 1)

GEOMETRY-mono 1 is a prospectively designed, multicenter, open-label, single arm Phase II study of oral cMET inhibitor (capmatinib) in adult patients with *EGFR* wild-type (wt), advanced NSCLC. The primary objective was to assess overall response rate (ORR) by a BIRC assessment to determine whether treatment with capmatinib is effective. Patients have been enrolled into multiple cohorts of the study, out of which the bridging study was focused on the fully-enrolled *MET* exon 14 deletion positive Cohorts 4 and 5b. Cohort 4 only enrolled pretreated (second and third line) *MET* exon 14 deleted patients, and Cohort 5b only enrolled treatment-naïve *MET* exon 14 deleted patients. Patients were screened for enrollment into Cohorts 4 and 5b for *MET* exon 14 deletion status using a *MET* exon 14 deletion reverse-transcriptase PCR (RT-PCR) CTA. After initial patient screening, clinical samples were stored for retrospective testing. GEOMETRY-mono 1 is an ongoing trial that was initiated on June 11, 2015 with first patient first visit (FPFV). Patients receive 400 mg of capmatinib orally twice daily in tablet form. Dose adjustments for capmatinib are permitted for safety concerns. Efficacy is evaluated every six weeks from the first day of treatment until RECIST 1.1 disease progression.

3.12.2 Summary of the Clinical Bridging Study

The safety and effectiveness of F1CDx for detecting SNVs and indels that lead to *MET* exon 14 skipping in NSCLC patients who may benefit from treatment with capmatinib was demonstrated in a retrospective analysis of samples from patients enrolled in the GEOMETRY-mono 1 trial. A bridging study was conducted to assess the clinical efficacy of F1CDx in identifying patients positive for SNVs and indels that lead to *MET* exon 14 skipping for treatment with capmatinib and the concordance between *MET* exon 14 deletion status tested with the CTA and F1CDx in the intent-to-test population. Retrospective testing with F1CDx was done for patients from Cohorts 4 and 5b, and a random selection of *MET* exon 14 deletion negative patients. The retrospective testing population consisted of 204 patients (78 *MET* exon 14 deletion positive patients, and 126 *MET* exon 14 deletion negative patient samples), originally tested by the *MET* exon 14 CTA for patient selection.

3.12.3 Safety Analysis

The F1CDx assay is not expected to directly cause actual or potential adverse effects, but test results may directly impact patient treatment risks.

3.12.4 Accountability of the PMA Cohorts

A total of 3036 patients were screened for trial eligibility from 152 investigational sites across 25 countries. 2551 patients within the original 3036 were screened for *MET* exon 14 deletion by the CTA. Within that screened population, 2295 patients produced valid positive and negative CTA results. As of April 15, 2019,

a total of 334 patients had been enrolled into all available cohorts. Of the patients whose samples produced valid CTA results, 97 were enrolled into Cohorts 4 and 5b of the GEOMETRY-mono 1 trial, with 69 and 28 patients respectively. *MET* exon 14 deletion negative patients were not enrolled in the GEOMETRY-mono 1 trial. Available samples from *MET* exon 14 deletion negative patients were evaluated for the bridging study, including 130 randomly selected CTA-negative patients. Out of the 130 CTA-negative samples, 93 were randomly assigned to Cohort 4 and 37 to Cohort 5b. Of the 227 positive and negative samples (97 positive and 130 negative), retrospective testing with F1CDx was performed for 204 CTA-tested patient samples that met the F1CDx sample testing criteria (78 positive and 126 negative). The F1CDx testing yielded 198 CDx-evaluable results and six (6) invalid results for the CDx and CTA concordance analysis.

Sensitivity analyses were conducted with all 227 samples to determine the impact of missing F1CDx results on concordance and efficacy results, which included 19 positive patient samples not tested due to failing to meet the F1CDx minimum tissue sample requirements, laboratory error and/or not meeting quality control metrics.

3.12.5 Clinical Concordance

The primary concordance analysis was conducted on 204 samples (78 positive and 126 negative). Agreement between F1CDx and the CTA was demonstrated. The point estimates of PPA, NPA and OPA between F1CDx and the CTA, shown in Table 46, were calculated with and without invalid CDx results, using the CTA results as reference for the CTA-enrolled patients.

Table 46. Agreement between F1CDx and CTA based on CTA results in combined cohorts by F1CDx sample requirements.

Measure of agreement	Without CDx "Invalid"		With CDx "Invalid"		
	Percent agreement % (n/N)	95% CI (1)	Percent agreement % (n/N)	95% CI (1)	
Cohort 4 and Cohort 5b	PPA	98.6 (72/ 73)	(92.6, 100)	92.3 (72/ 78)	(84.0, 97.1)
	NPA	100 (125/125)	(97.1, 100)	99.2 (125/126)	(95.7, 100)
	OPA	99.5 (197/198)	(97.2, 100)	96.6 (197/204)	(93.1, 98.6)

N: The total number of patients. It is the denominator for percentage (%) calculation.

n: Number of patients with agreement between CTA and CDx.

(1) The 95% CI calculated using Clopper-Pearson method

3.12.6 Efficacy Evaluation

GEOMETRY- mono 1 clinical efficacy results

The GEOMETRY-mono 1 clinical trial met the primary objective, demonstrating a high ORR as assessed by BIRC. Treatment with capmatinib was considered efficacious in both Cohort 4 (second and third line) and Cohort 5b (treatment-naive) as demonstrated by an ORR per BIRC of 40.6% (95% CI: 28.9, 53.1) and of 67.9% (95% CI: 47.6, 84.1), respectively (Table 47 below). Robustness of the data was further confirmed by the supportive analysis of ORR by Investigator assessment, ORR for the PFS and for key subgroups.

Table 47. Treatment-naïve and previously treated *MET*-skipping positive locally advanced or metastatic NSCLC - efficacy results in patients treated with capmatinib in GEOMETRY-mono 1

Efficacy Parameter	Previously Treated (Cohort 4) N = 69	Treatment-Naïve by (Cohort 5b) N = 28
Overall Response Rate^a, % (95% CI)^b	40.6 (28.9, 53.1)	67.9 (47.6, 84.1)
Complete Response (CR), n (%)	0	3.6%
Partial Response (PR), n (%)	40.6%	64.3%

^a Determined by RECIST v1.1.
^b Clopper and Pearson exact binomial 95% CI.

Clinical efficacy results in the CDx-positive population

Clinical utility of F1CDx was evaluated by estimation of clinical efficacy in the CTA-enrolled *MET* exon 14 deletion positive patient population, as assessed by the primary objective of ORR by BIRC. Baseline demographic and disease characteristics were compared between the CDx evaluable and CDx unevaluable within all enrolled CTA-positive patients in Cohorts 4 and 5b. Clinical efficacy of capmatinib in patients with SNVs and indels that lead to *MET* exon 14 skipping with valid CDx results and after imputing missing CDx results were similar between the CDx-positive and CTA-positive patient groups in the GEOMETRY-mono 1 trial. Table 48 shows the efficacy results in CTA enrolled CDx-positive patients, while detailed efficacy results are available in Tables 16 and 17 of the SSED.

Table 48. Summary of clinical efficacy results by test method and sample set

Test Method	Cohort 4 ORR with 95% CI	Cohort 5b ORR with 95% CI
F1CDx	44.2% (30.6 – 58.7%)	70% (45.7 – 88.1 %)
CTA	40.6% (28.9 – 53.1%)	67.9% (47.6 – 84.1%)

3.12.7 Conclusions

The data from this study support reasonable assurance of the safety and effectiveness of the F1CDx assay when used to aid clinicians in identifying NSCLC patients with SNVs and indels that lead to *MET* exon 14 skipping who may be eligible for treatment with capmatinib.

3.13 Clinical evaluation of HRR gene alterations for treating prostate cancer patients with olaparib

The clinical performance of F1CDx for determination of the mutation status of the HRR gene panel was established based on confirmed FMI F1CDx subgroup results, which were derived from tumor analysis results using the CLIA HRR CTA in the clinical study D081DC00007 (PROfound).

Study Design

PROfound was a Phase III, randomised, open-label, multicentre trial to assess the efficacy and safety of olaparib monotherapy in patients with metastatic castration-resistant prostate cancer (mCRPC) that have qualifying homologous recombination repair (HRR) gene mutations that were predicted to be deleterious or suspected deleterious (known or predicted to be detrimental/lead to loss of function) who have failed prior treatment with a new hormonal agent (NHA).

Patients were randomised in a 2:1 ratio to the treatments as specified below:

- Olaparib tablets orally 300 mg bd
- Investigators choice of NHA with either enzalutamide 160 mg orally once daily (od) or abiraterone acetate 1000 mg orally qd with prednisone 5 mg orally bd (prednisolone was permitted for use instead of prednisone, if necessary)

Eligible patients were those with HRRm mCRPC, who had progressed following prior treatment with an NHA. All patients must have had a qualifying HRR mutation assessed via the FMI CLIA HRR CTA to be randomised. Qualifying HRR gene mutations were *BRCA1*, *BRCA2* and *ATM* for Cohort A, and *BARD1*, *BRIP1*, *CDK12*, *CHEK1*, *CHEK2*, *FANCL*, *PALB2*, *PPP2R2A*, *RAD51B*, *RAD51C*, *RAD51D* and *RAD54L* for Cohort B.

Note: Although patients with PPP2R2A gene mutations were enrolled in the trial, Lynparza is not indicated for the treatment of patients with this gene mutation because of lack of response, and a numerical decrement in both rPFS and OS compared to enzalutamide or abiraterone.

Safety Analysis

The F1CDx assay is not expected to directly cause actual or potential adverse effects, but test results may directly impact patient treatment risks.

Efficacy Evaluation

PROfound met its primary objective, demonstrating a statistically significant improvement in rPFS as assessed by BICR with olaparib 300 mg bd compared with investigators choice of NHA in Cohort A. Specifically, the PROfound efficacy data with olaparib demonstrated:

- A statistically significant improvement in rPFS as assessed by BICR with olaparib 300 mg bd compared with investigators choice of NHA in Cohort A, with a 66% reduction in the risk of BICR-confirmed radiological disease progression or death and a prolongation of median progression free interval of 3.8 months with olaparib vs investigators choice of NHA. The rPFS outcome in the confirmed FMI F1CDx subgroup (HR 0.33 [95% CI 0.24, 0.46]) was consistent with the Full Analysis Set (FAS) (HR 0.34 [95% CI 0.25, 0.47]).

Table 49. Summary of analysis of rPFS based on BICR (Cohort A).

Analysis group:	Full Analysis Set		Confirmed FMI F1CDx Subgroup	
	Olaparib 300 mg bd (N=162)	Investigators choice of NHA (N=83)	Olaparib 300 mg bd (N=157)	Investigators choice of NHA (N=83)
n (%) of events ^a	106 (65)	68 (82)	101 (64)	68 (82)
Treatment effect				
Median rPFS (95% CI) [months]	7.4 (6.24, 9.33)	3.6 (1.91, 3.71)	7.4 (6.87, 9.33)	3.6 (1.91, 3.71)
HR (95% CI) ^b	0.34 (0.25, 0.47)		0.33 (0.24, 0.46)	
2-sided p-value ^c	<0.0001		<0.0001	

^a Progression, as assessed by BICR, was defined by RECIST 1.1 and/or PCWG-3 or death (by any cause in the absence of progression) regardless of whether the patient withdrew from randomised therapy or received another anticancer therapy prior to progression.

^b The HR and CI were calculated using a Cox proportional hazards model adjusted for the variables selected in the primary pooling strategy (prior taxane use and measurable disease in Cohort A). The Efron approach was used for handling ties. An HR <1 favours olaparib 300 mg bd.

^c The analysis was performed using the log-rank test stratified by the variables selected in the primary pooling strategy (prior taxane use and measurable disease in Cohort A) using the Breslow method for handling ties.

bd twice daily; BICR blinded independent central review; CI confidence interval; FAS full analysis set; HR hazard ratio; NHA new hormonal agent; PCWG-3 Prostate Cancer Working Group 3; RECIST Response Evaluation Criteria in Solid Tumours; rPFS radiological progression-free survival.

- There was a statistically significant improvement in confirmed radiological ORR by BICR for patients in Cohort A with measurable disease at baseline in the olaparib arm compared with the investigators' choice of NHA arm. The efficacy in the confirmed FMI F1CDx subgroup showed a similar performance as compared to the Full Analysis Set.

Table 50. Confirmed radiological objective response rate, logistic regression based on BICR (EFR; Cohort A).

Analysis group	Treatment group	N	Number (%) of patients with response ^a	Comparison between groups
				2-sided p-value ^b
Full Analysis Set	Olaparib 300 mg bd	84	28 (33.3)	<0.0001
	Investigators choice of NHA	43	1 (2.3)	
Confirmed FMI F1CDx Subgroup	Olaparib 300 mg bd	84	27 (33.8)	<0.0001
	Investigators choice of NHA	43	1 (2.3)	

^a Radiological objective response rate determined based on BICR assessed RECIST 1.1 and bone scan data (using all scans regardless of whether they were scheduled or not) in patients with measurable disease. Response required confirmation. Radiological objective response rate compared using logistic regression (PROC GENMOD) adjusting for previous taxane use as a covariate.

^b Where the number of patients with a response was ≥ 5 , a 1-sided p-value was calculated based on twice the change in log-likelihood resulting from the addition of the treatment factor to the model that contains the specified covariates. Where the number of patients with a response was < 5 , the 2-sided p-value was calculated based on the mid p-value modification of the Fisher's exact test.

- There was a statistically significant improvement in rPFS as assessed by BICR for olaparib-treated patients compared with investigators choice of NHA-treated patients in Cohort A+B, with a 51% reduction in the risk of radiological disease progression or death and a prolongation of median progression-free interval of 2.3 months with olaparib vs investigators choice of NHA (HR=0.49; 95% CI 0.38, 0.63; $p < 0.0001$; median rPFS 5.8 months vs 3.5 months, respectively, for FAS and confirmed FMI F1CDx subgroup).

Table 51. Summary of analysis of rPFS based on BICR (Cohort A+B).

Analysis group:	Full Analysis Set		Confirmed FMI F1CDx Subgroup	
	Olaparib 300 mg bd (N=256)	Investigators choice of NHA (N=131)	Olaparib 300 mg bd (N=248)	Investigators choice of NHA (N=128)
n (%) of events ^a	180 (70.3)	99 (75.6)	172 (69.4)	96 (75.0)
Treatment effect				
Median rPFS (95% CI) [months]	5.8 (5.52, 7.36)	3.5 (2.20, 3.65)	6.2 (5.52, 7.36)	3.5 (2.10, 3.65)
HR (95% CI) ^b	0.49 (0.38, 0.63)		0.49 (0.38, 0.63)	
2-sided p-value ^c	<0.0001		<0.0001	

^a Progression, as assessed by BICR, was defined by RECIST 1.1 and/or PCWG-3 or death (by any cause in the absence of progression) regardless of whether the patient withdrew from randomised therapy or received another anticancer therapy prior to progression.

^b The HR and CI were calculated using a Cox proportional hazards model adjusted for the variables selected in the primary pooling strategy (prior taxane use and measurable disease in Cohort A+B). The Efron approach was used for handling ties. An HR < 1 favours olaparib 300 mg bd.

^c The analysis was performed using the log-rank test stratified by the variables selected in the primary pooling strategy (prior taxane use and measurable disease in Cohort A+B) using the Breslow method for handling ties.

bd twice daily; BICR blinded independent central review; CI confidence interval; FAS full analysis set; HR hazard ratio; NHA new hormonal agent; PCWG-3 Prostate Cancer Working Group 3; RECIST Response Evaluation Criteria in Solid Tumours; rPFS radiological progression-free survival.

- In Cohort A, the interim OS data indicate a trend for OS benefit in olaparib -treated patients compared with investigators choice of NHA-treated patients, with a median OS improvement of 3.4 months in the olaparib- arm vs the investigators choice of NHA arm (HR=0.64; 95% CI 0.43, 0.97; p=0.0173; median OS 18.5 months vs 15.1 months, respectively).
- The olaparib safety and tolerability profile in this study was consistent with that observed in previous studies of olaparib.

3.14 Clinical Evaluation of pembrolizumab in TMB-H solid tumors Summary of the Clinical Study – KEYNOTE-158

The clinical performance of F1CDx for detecting TMB-H (defined as TMB \geq 10 mutations per megabase) and the efficacy of KEYTRUDA (pembrolizumab) were investigated in a prospectively-planned retrospective analysis of 10 cohorts (A through J) of patients with various previously treated unresectable or metastatic solid tumors with high tumor mutational burden (TMB) who were enrolled in a multicenter, non-randomized, open-label trial, KEYNOTE-158 (NCT02628067). The trial excluded patients who previously received an anti-PD-1 or other immune-modulating monoclonal antibody, or who had an autoimmune disease, or a medical condition that required immunosuppression. Patients received KEYTRUDA 200 mg intravenously every 3 weeks until unacceptable toxicity or documented disease progression. Assessment of tumor status was performed every 9 weeks for the first 12 months and every 12 weeks thereafter.

The statistical analysis plan pre-specified ≥ 10 and ≥ 13 mutations per megabase using F1CDx as cutpoints to assess TMB. Testing of TMB was blinded with respect to clinical outcomes. The major efficacy outcome measures were ORR and DoR in the patients who have received at least one dose of KEYTRUDA as assessed by BICR according to RECIST v1.1, modified to follow a maximum of 10 target lesions and a maximum of 5 target lesions per organ.

In KEYNOTE-158, 1,050 patients (Cohorts A through J) were included in the efficacy analysis population. TMB was analysed in the therapeutic efficacy (TE) subset of 790 patients with sufficient tissue for testing based on testing requirements for the investigational F1CDx assay. Of the 790 patients, 102 (13%) had tumors identified as TMB-H (defined as a TMB \geq 10 mutations per megabase). Among the 102 TMB-H patients, the study population characteristics were: median age of 61 years (range: 27 to 80), 34% age 65 or older; 34% male; 81% White; and 41% ECOG PS of 0 and 58% ECOG PS of 1. TMB was also analysed in the device validation (DV) population of 719 patients using the final F1CDx assay. Of the 719 patients, 91 (13%) had tumor identified as TMB-H (\geq 10 mutations per megabase) and the study population characteristics were: median age of 60 years (range: 27 to 80), 35% age 65 or older; 34% male; 81% White; and 41% ECOG PS of 0 and 58% ECOG PS of 1.

Efficacy results for the therapeutic efficacy (TE) (n=102) and device validation (DV) (n=91) populations are summarized in Table 52.

Table 52. Efficacy results for patients with TMB-H (\geq 10 mut/Mb) cancer in KEYNOTE-158.

Endpoint	KEYTRUDA 200 mg every 3 weeks	
	Therapeutic Efficacy Population n=102*	Device Validation Population n=91*
Objective Response Rate		
ORR (95% CI)	29% (21, 39)	33% (24, 44)
Complete response rate	4%	4%
Partial response rate	25%	29%
Duration of Response		
Median in months (range)	NR (2.2+, 34.8+)†	NR (2.2+, 34.8+)†
% with duration ≥6 months	87%	87%
% with duration ≥12 months	57%	57%
% with duration ≥24 months	50%	50%

* Median follow-up time of 11.1 months for TE population, and 13.4 months for DV population.

† Based on patients (n=30) with a response by independent review

+ Denotes ongoing
NR = not reached

ORR was assessed by tumor type, and the results were similar in the TE and DV populations. Efficacy results per tumor type are shown for the TE and DV populations in Tables 53 and 54, respectively. ORR was generally higher in the TMB-H population for most tumor types than in the non-TMB-H population.

Table 53. Summary of best objective response per tumor type in TE population.

Tumor Type*	TMB ≥10 mut/Mb				TMB <10 mut/Mb				ORR Ratio‡ TMB ≥10 mut/Mb vs. TMB <10 mut/Mb
	N	n	%	95% CI†	N	n	%	95% CI†	
Overall	102	30	29	(21, 39)	688	43	6	(5, 8)	4.7
Anal	14	1	7	(0.2, 34)	75	8	11	(5, 20)	0.7
Neuroendocrine	5	2	40	(5, 85)	82	1	1	(0, 7)	32.8
Endometrial	15	7	47	(21, 73)	67	4	6	(2, 15)	7.8
Cervical	16	5	31	(11, 59)	59	7	12	(5, 23)	2.6
Vulvar	12	2	17	(2, 48)	59	2	3	(0, 12)	4.9
Small Cell Lung	34	10	29	(15, 47)	42	4	10	(3, 23)	3.1
Mesothelioma	1	0	0	(0, 98)	84	9	11	(5, 19)	0.0
Thyroid	2	2	100	(16, 100)	78	3	4	(1, 11)	26.0
Salivary	3	1	33	(1, 91)	79	3	4	(1, 11)	8.8

* No TMB-H patients were identified in the cholangiocarcinoma cohort

† Based on binomial exact confidence interval method.

‡ ORR ratios were calculated prior to rounding the objective response values shown in this table

Table 54. Summary of best objective response per tumor type in DV population.

Tumor Type	TMB ≥10 mut/Mb				TMB <10 mut/Mb				ORR Ratio TMB ≥10 mut/Mb vs. TMB <10 mut/Mb
	N	n	%	95% CI†	N	n	%	95% CI†	
Overall	91	30	33	(24, 44)	628	41	7	(5, 9)	5.0
Anal	14	1	7	(0.2, 34)	73	8	11	(5, 20)	0.7
Neuroendocrine	5	2	40	(5, 85)	73	1	1	(0, 7)	29.2

Endometrial	15	7	47	(21, 73)	64	3	5	(1, 13)	10.0
Cervical	15	5	33	(12, 62)	52	6	12	(4, 23)	2.9
Vulvar	10	2	20	(3, 56)	52	2	4	(0.5, 13)	5.2
Small Cell Lung	26	10	38	(20, 59)	30	4	13	(4, 31)	2.9
Mesothelioma	1	0	0	(0, 98)	80	9	11	(5, 20)	0.0
Thyroid	2	2	100	(16, 100)	75	3	4	(1, 11)	25.0
Salivary	3	1	33	(1, 91)	74	3	4	(1, 11)	8.2

* No TMB-H patients were identified in the cholangiocarcinoma cohort

† Based on binomial exact confidence interval method.

‡ ORR ratios were calculated prior to rounding the objective response values shown in this table

The KEYNOTE-158 results indicate that pembrolizumab monotherapy provides clinically meaningful ORR and DoR in previously treated participants with TMB-H solid tumors across cancer types who have no satisfactory alternative treatment options.

3.15 Clinical evaluation of VITRAKVI (larotrectinib) in patients with solid tumors with *NTRK1*, *NTRK2*, *NTRK3* fusions

Summary of Clinical Studies

The clinical validity of FoundationOne[®]CDx (F1CDx) for detecting *NTRK1*, *NTRK2*, or *NTRK3* fusions in patients with solid tumors who may benefit from treatment with larotrectinib was demonstrated in a clinical bridging study that consisted of the retrospective analysis of specimens from patients enrolled in the LOXO-TRK-14001 (Bayer 20288, NCT02122913), -15002 (Bayer 20289, NAVIGATE, NCT02576431), and -15003 (Bayer 20290, SCOUT, NCT02637687) clinical trials (referred to as 14001, 15002, and 15003, respectively) supplemented with *NTRK* fusion negative samples from the FMI clinical archive. Study 14001 is an on-going, multicenter, open-label, Phase 1 dose escalation study in adult patients with advanced solid tumors (all comers) unselected for *NTRK* gene fusion cancer. Following the dose escalation portion of the study, a dose expansion was initiated for patients with documented TRK fusion cancer and for patients who the Investigator believed might benefit from a highly selective TRK inhibitor. Study 15002 is an on-going multi-center, open-label, Phase 2 “basket” study in patients age 12 and older with recurrent advanced solid tumors with a documented *NTRK* gene fusion as assessed by an outside laboratory. Finally, Study 15003 is an on-going multi-center, open-label, Phase 1/2 study in pediatric patients aged from birth to 21 years with advanced solid or primary central nervous system (CNS) tumors.

NTRK fusion status to determine patient eligibility for enrollment was performed using local clinical trial assay (LCTAs) that included DNA next generation sequencing (NGS), RNA NGS, fluorescent in situ hybridization (FISH), and reverse transcriptase- polymerase chain reaction (RT-PCR) methods. The majority of 105 clinical trial patients with known *NTRK* fusion status enrolled into the trials had been tested with NGS methods (92%); 51% of the 105 patients had been tested with DNA NGS methods and 41% with RNA NGS methods. Of the 105 clinical trial patients, 78 patients were *NTRK* fusion positive and 27 were *NTRK* fusion negative. The assessment of efficacy of larotrectinib was based on the first 55 patients with solid tumors with an *NTRK* gene fusion enrolled across the three clinical trials. The primary endpoint was overall response rate (ORR) according to independent review committee assessment using RECIST v1.1 criteria. The ORR of the 55 patient set was 75%, 95% CI: [61%, 85%].

Accountability of the PMA Cohort

Of the 78 *NTRK* fusion positive patients and 27 *NTRK* fusion negative patients enrolled in 14001, 15002, and 15003, 45 patients and 24 patients, respectively, had samples available for testing with F1CDx for a total of 69 samples. Of the 69 samples, 67 samples had valid results and were used to support the clinical concordance analysis. Two(2) samples had invalid results due to failing F1CDx input criteria or low tumor purity. Of the 55 *NTRK* fusion positive patients in the efficacy set, 32 had samples available testing with F1CDx. F1CDx testing yielded 31 valid results to support the F1CDx efficacy analysis. One sample was invalid due to failing F1CDx input criteria.

In addition to clinical trial samples, 206 supplemental *NTRK* fusion negative samples as determined by the DNA NGS FoundationOne LDT were provided from the FMI clinical archive to support the clinical concordance study. Of these 206 samples that were re-tested on F1CDx, 203 samples had valid results.

FoundationOne® CDx Clinical Bridging Study for *NTRK*

A clinical bridging study was conducted to assess the clinical effectiveness of F1CDx in identifying *NTRK1*, *NTRK2*, or *NTRK3* fusion positive patients for treatment with larotrectinib, and to assess the concordance between *NTRK* fusion positive samples tested with the LCTAs and F1CDx. F1CDx was used to retrospectively test the available patient samples from studies 14001, 15002, and 15003 (N = 69) and the supplemental *NTRK* fusion negative samples (N = 206).

Safety Analysis

The F1CDx assay is not expected to directly cause actual or potential adverse effects, but test results may directly impact patient treatment risks. Refer to Drugs@FDA for complete safety information on VITRAKVI® (larotrectinib)

Effectiveness Results Concordance Analysis

The concordance analysis between the F1CDx and the LCTAs using the clinical trial samples and supplemental negatives is shown in Table 55.

Table 55: Concordance between the F1CDx and LCTA methods for detection of *NTRK* gene fusions based on the LCTA results (all patients tested by CDx)

Measure of Agreement	Excluding CDx invalid results		Including CDx invalid results	
	% Agreement (N)	95% CI (a)	% Agreement (N)	95% CI (a)
Positive percent agreement	84.1% (37/44)	69.9% -93.4%	82.2% (37/45)	67.9% -92.0%
Negative percent agreement	100.0% (226/226)	98.4% -100.0%	98.3% (226/230)	95.6% -99.5%
Overall percent agreement	97.4% (263/270)	94.7% -99.0%	95.6% (263/275)	92.5% -97.7%

Abbreviations: CDx = Companion Diagnostic; CI = Confidence Interval; LCTA= Local Clinical Trial Assay; *NTRK* = Neurotrophic Tyrosine Kinase.

The LCTA inferred *NTRK3* gene fusions were considered fusion positive.

a The 95% CI was calculated using the Clopper-Pearson exact method.

A sensitivity analysis against the 34 missing CDx results was conducted to assess the robustness of the agreement analysis. Missing CDx results for the LCTA fusion positive patients were imputed using a logistic regression model including 10 covariates (race, ethnicity, age group, stage of disease at initial diagnosis, prior cancer systemic treatments, prior cancer related surgery, ECOG performance status, *NTRK* fusion gene, LCTA method sample substrate, and binary clinical response to larotrectinib). Agreement estimates, including the imputed values, were PPA= 78.3%, 95% CI [64.4%, 89.9%] and NPA=100% (Table 56). The method of calculation for the 95% confidence interval accounted for both within and between imputation variance.

Table 56. Concordance between the CDx and LCTA methods for detection of *NTRK* gene fusions including imputed values in LCTA fusion positive patients with missing CDx results

Measure of Agreement	% Agreement	95% CI (a)
PPA	78.3%	64.4%, 89.9%
NPA	100.0%	100.0%, 100.0%
OPA	94.4%	90.5%, 97.4%

a The 95% CI was calculated based on multiple imputation (MI) Boot pooled sample method.

The F1CDx assay showed high concordance with the DNA NGS LCTA methods with PPA = 95%, 95% CI [75%, 100%] and NPA = 100%, 95% CI [98%, 100%] (Table 57).

Table 57. Concordance between the CDx and DNA NGS LCTA methods for detection of *NTRK* gene fusions based on LCTA results and excluding invalid results

Measure of Agreement	% Agreement (N)	95% CI ^(a)
PPA	95.0% (19/20)	75.1%, 99.9%
NPA	100.0% (221/221)	98.3%, 100.0%
OPA	99.6% (240/241)	97.7%, 100.0%

^a The 95% CI was calculated based on Clopper-Pearson exact method.

However, the positive concordance of F1CDx with RNA NGS methods was lower (PPA = 70%, 95% CI [46%, 88%]) (Table 58).

Table 58. Concordance between the CDx and RNA NGS LCTA methods for detection of *NTRK* gene fusions based on LCTA results and excluding invalid results

Measure of Agreement	% Agreement (N)	95% CI ^(a)
PPA	70.0% (14/20)	45.7%, 88.1%
NPA	100.0% (4/4)	39.8%, 100.0%
OPA	75.0% (18/24)	53.3%, 90.2%

^a The 95% CI was calculated based on Clopper-Pearson exact method.

F1CDx was concordant with FISH and RT-PCR based on testing of 5 samples (Table 59). Due to the low sample counts, agreement measures were not calculated.

Table 59. Contingency table comparing *NTRK* fusion detection results between the CDx and the FISH and RT-PCR LCTA methods (all patients tested by CDx)

F1CDx result by test method	LCTA positive	LCTA negative
FISH		
CDx Positive	3	0
CDx Negative	0	1
Total	3	1
RT-PCR		
CDx Positive	1	0
CDx Negative	0	0
Total	1	0

FISH = Fluorescence in Situ Hybridization; RT-PCR = Reverse Transcriptase-Polymerase Chain Reaction.

A total of 7 of the 275 samples tested with the F1CDx assay showed discordant results between F1CDx and the LCTAs. All 7 discordant results were *NTRK* fusion positive by the LCTA and fusion negative by F1CDx. Of the seven (7) discordant results, six (6) had been tested with an RNA NGS LCTA method and one (1) with an DNA NGS LCTA method.

The discordances between the RNA NGS LCTA methods and F1CDx can be explained by differences in technology used to detect *NTRK1/2/3* fusions, as well as an expected degree of measurement error by the LCTAs and F1CDx. *NTRK* often presents complex genomic rearrangement events with a variety of breakpoints spanning multiple introns. This complexity of rearrangement events presents certain limitations for targeted DNA sequencing. F1CDx was designed to focus on hotspot introns that are repeatedly described in the literature, which means rare and complex breakpoints may not be captured by F1CDx baiting. The DX1 bait-set used by the F1CDx assay includes the coding regions of *NTRK1*, *NTRK2*, and *NTRK3* and select introns from these genes, however no introns within *NTRK3* are baited and the *NTRK1* intron 8, and *NTRK2* intron 12 are not fully baited. While the most common fusion partner of *NTRK3*, *ETV6*,

has several introns baited which allows for detection *ETV6-NTRK3* fusions, *EVT6* intron 5 is also not fully baited. A portion of fusion events between these two genes are likely being undetected as a result of DX1 also not baiting intron 4 of *ETV6*.

Of the seven (7) discordant patients, four (4) patients had complete or partial response, supporting that these four (4) samples were most likely true positives. Investigation findings concluded that F1CDx did not detect the fusion events in six (6) of the discordances for one of two reasons: 1) F1CDx does not bait the intron where the breakpoint occurred, or 2) the rearrangement event was too complex to be fully baited by F1CDx, and therefore the full picture of the event was not captured. The remaining one (1) discordant case could have been explained by time of sample collection and testing, since the sample tested by F1CDx was from a sample collected at a different timepoint than used for the LCTA test.

Clinical Efficacy Results

Clinical effectiveness of F1CDx was evaluated by estimation of clinical efficacy in the F1CDx-positive, LCTA-positive population. Clinical outcome was assessed by independent review committee using RECIST 1.1 criteria. Efficacy of larotrectinib in the F1CDx positive, LCTA-positive population was 77% (95% CI: [56%, 91%]) overall response rate (see Table 60). This is comparable to the efficacy for the NDA filing, where larotrectinib demonstrated an estimated 75% (95% CI: [61%, 85%]) overall response rate in the NDA efficacy population. Of the 26 F1CDx-positive patients in the efficacy set, six (6) (23%) patients had achieved a complete response and 14 (54%) had received a partial response with larotrectinib therapy (see Table 60).

Table 60. Primary efficacy results: the best overall response and overall response rate for *NTRK* fusion positive patients by LCTA and CDx results in the efficacy analysis set

Clinical outcome	LCTA fusion positive (N=55)	CDx fusion positive and LCTA fusion positive (N=26)	CDx fusion Negative and LCTA fusion positive (N=5)	CDx fusion results missing and LCTA fusion positive (N=24)
ORR% (95% CI^(a))	75% (61%, 85%)	77% (56%, 91%)	80% (28%, 99%)	71% (49%, 87%)
Complete response	12 (22%)	6 (23%)	2 (40%)	4 (17%)
Partial response	29 (53%) ^b	14 (54%)	2 (40%)	13 (54%) ^b
Duration of Response^(c)	N=41	N=20	N=4	N=17
Range (months)	1.6, 33.2	1.6, 20.3	3.7, 23.6	2.7, 33.2
% with duration ≥ 6 months	73.2%	80.0%	50.0%	70.6%
% with duration ≥ 9 months	63.4%	65.0%	50.0%	64.7%
% with duration ≥ 12 months	39.0%	25.0%	50.0%	52.9%

^a The 95% confidence interval was calculated using the Clopper-Pearson exact method.

^b Includes one pediatric patient with unresectable infantile fibrosarcoma who underwent resection following partial response and who remained disease-free at data cutoff.

^c Includes patients with ongoing response after data cutoff.

Twenty-four (24) patients have missing CDx results (i.e., 43.6% of the PAS population have missing results). Sensitivity analysis against the 24 missing CDx results was conducted to assess the robustness of the clinical efficacy analysis for the F1CDx positive patients. Missing CDx results for

the LCTA fusion positive patients in the efficacy set were imputed 100 times using a logistic regression model including 9 covariates based on the missing at random (MAR) assumption. Covariates identified included covariates imbalanced between the CDx evaluable and CDx non-evaluable sets, covariates associated with the F1CDx results and covariates associated with patient clinical response to larotrectinib. 9 covariates were used in the imputation model for the efficacy sensitivity analysis: race, ethnicity, age group, gender, stage of disease at initial diagnosis, ECOG performance status, *NTRK* fusion gene, LCTA method sample substrate, and binary clinical response to larotrectinib. Clinical efficacy, including the imputed CDx results, was ORR=74%, 95% CI [59%, 89%] (Table 61) and was similar to the results of the primary efficacy analysis (ORR=77%, 95% CI [56%, 91%]) (Table 49). However, it should be noted that the clinical effectiveness of F1CDx to identify patients with solid tumors with *NTRK1*, *NTRK2* or *NTRK3* fusions who may benefit from larotrectinib treatment is based on ~56% of the efficacy population.

Table 61. Sensitivity analysis for overall response rate by CDx result for NTRK fusion positive patients including imputed values for missing CDx results in the efficacy analysis set

Clinical Outcome	CDx fusion positive and LCTA fusion positive	CDx fusion negative and LCTA fusion positive
ORR% (95% CI ^(a))	74% (59% - 89%)	78% (46% - 100%)

^a The 95% confidence interval was calculated based on MI Boot pooled sample method.

Sensitivity analysis was performed to estimate ORR in the total F1CDx positive population including the F1CDx positive, LCTA positive and the F1CDx positive, LCTA negative subpopulations. To assess the potential impact of the F1CDx positive, LCTA negative portion of the F1CDx positive intended use population on clinical effectiveness, 206 *NTRK* negative samples by the FoundationOne LDT were selected from the FMI clinical archive along with 24 *NTRK* negative clinical trial samples available for testing were used to obtain a NPA that was representative for the LCTAs used to enroll patients in the larotrectinib trials. Since the estimated NPA (PPV) is 100%, the ORR for the F1CDx positive population is the same as the ORR for the F1CDx positive and LCTA positive population. However the NPA estimate between F1CDx and LCTA is subject to uncertainty and could be biased given that the majority of the *NTRK* fusion negative patients, in both the full population and those whose samples were available for testing with F1CDx had been tested using DNA NGS methods (>70%). FoundationOne LDT was the most commonly used DNA based NGS method that was used for *NTRK* fusion status determination for patients in the larotrectinib clinical trials. The same assay was also used to selected the supplemental negative samples in the clinical bridging study as the representative LCTA. Therefore the estimated NPA could be subject to bias.

Sensitivity analysis to determine the minimum PPV that will lead to an ORR of 30% at the lower bound of the two-sided 95% confidence interval for the CDx positive population was performed. This analysis was conducted to determine the NPA corresponding to this tipping point PPV by assuming fixed prevalence of *NTRK* fusion (0.32%)⁷ and PPA (84%) observed from the concordance analysis to demonstrate the robustness of the study results.

For each value of c (the scaling factor for the assumed ORR (LCTA negative/F1CDx positive)), the tipping point PPV that led to an ORR of the F1CDx positive population with the lower bound of the two-sided 95% confidence interval at 30% was determined. When c is greater than or equal to 0.85, indicating the ORR in the LCTA negative/F1CDxpositive population is close to the ORR in the LCTA positive/F1CDxpositive population, the two-sided 95% lower confidence limit (LCL) of ORR is always greater than 30% so there is no tipping point of PPV. At all values of PPV (and NPA), the two-sided 95% LCL is > 30%. At c values between 0 and 0.8, a tipping point PPV ranges from 99.5% to 88.6% and NPA ranges from 100% to 99.97%.

Conclusions

The data from this study support reasonable assurance of the safety and effectiveness of the F1CDx assay when used to aid clinicians in identifying solid tumor patients harboring *NTRK1*, *NTRK2*, or *NTRK3* fusions that may be treated with VITRAKVI® larotrectinib.

4. References

1. Li M. Statistical Methods for Clinical Validation of Follow-On Companion Diagnostic Devices via an External Concordance Study, *J Biopharm Stat* 26:6, 1067-107
2. Kimura H., Ohira T., Uchida O., et al. Analytical performance of the cobas *EGFR* mutation assay for Japanese non-small-cell lung cancer. *Lung Cancer* 83, 329-333 (2014).
3. Lopez-Rios F., Angulo B., Gomez B., et al. Comparison of molecular testing methods for the detection of *EGFR* mutations in formalin-fixed paraffin-embedded tissue specimens of non-small cell lung cancer. *J Clin Pathol* 66, 381–385 (2013).
4. Wong AT, To RM, Wong CL, et al. Evaluation of 2 Real-Time PCR Assays for In Vitro Diagnostic Use in the Rapid and Multiplex Detection of *EGFR* Gene Mutations in NSCLC. *Diagn Mol Pathol* 22, 138-43 (2013).
5. Press et al., HER2 Gene Amplification Testing by Fluorescent In Situ Hybridization (FISH): Comparison of the ASCO-College of American Pathologists Guidelines With FISH Scores Used for Enrollment in Breast Cancer International Research Group Clinical Trials, *J Clin Oncol* 34:3518-3528, 2016
6. Dowsett, M. et al, Disease-Free Survival According to Degree of HER2 Amplification for Patients Treated with Adjuvant Chemotherapy With or Without 1 Year of Trastuzumab: The HERA Trial, *J Clin Oncol* 27:2962-2969, 2009
7. Okamura R, Boichard A, Kato S, Sicklick JK, Bazhenova L, Kurzrock R. Analysis of NTRK Alterations in Pan-Cancer Adult and Pediatric Malignancies: Implications for NTRK Targeted Therapeutics. *JCO Precis Oncol*. 2018;2018:10.1200/PO.18.00183.

Revision Table

Revision Number	Reason for Change
1	Initial Release.
2	Updated to reflect two approved indications: (1) indication in NSCLC for EGFR exon 19 deletions and EGFR exon 21 L858R alterations in association with osimertinib and (2) indication in breast cancer for PIK3CA alterations in association with alpelisib.
3	Updates include: Addition of Section 3.10 Clinical Bridging Study data to support PIK3CA indication in breast cancer, addition of Summary of Clinical Concordance Study Table 3.7., and revision of table headers within Section 2.1-2.3 for additional clarity.
4	Update to reflect approved indication in cholangiocarcinoma for <i>FGFR2</i> fusions and select rearrangements associated with pemigatinib.

5	Updated to reflect approved indication in NSCLC for <i>MET</i> single nucleotide variants (SNVs) and indels that lead to <i>MET</i> exon 14 skipping in association with capamatinib.
6	Updated to reflect approved indication in prostate cancer for HRR gene alterations associated with olaparib.
7	Updated to reflect approved indication in pan-tumor cancer for TMB \geq 10 mutations per megabase associated with pembroluzimab.
8	Updated to reflect approved indication in pan-tumor cancer for <i>NTRK1/2/3</i> associated with larotrectinib.

PATIENT

DISEASE Unknown primary malignant neoplasm
NAME Not Given
DATE OF BIRTH Not Given
SEX Not Given
MEDICAL RECORD # Not Given

PHYSICIAN

ORDERING PHYSICIAN Not Given
MEDICAL FACILITY Not Given
ADDITIONAL RECIPIENT Not Given
MEDICAL FACILITY ID Not Given
PATHOLOGIST Not Given

SPECIMEN

SPECIMEN SITE Not Given
SPECIMEN ID Not Given
SPECIMEN TYPE Not Given
DATE OF COLLECTION Not Given
SPECIMEN RECEIVED Not Given

Companion Diagnostic (CDx) Associated Findings

GENOMIC FINDINGS

NTRK1 TPM3-NTRK1 fusion

FDA-APPROVED THERAPEUTIC OPTIONS

Vitakvi® (Larotrectinib)

For Microsatellite Instability (MSI) results, confirmatory testing using a validated orthogonal method should be performed.

OTHER ALTERATIONS & BIOMARKERS IDENTIFIED

Results reported in this section are not prescriptive or conclusive for labeled use of any specific therapeutic product. See professional services section for additional information.

Microsatellite status MS-Stable[§]

CDKN2A/B loss

Tumor Mutational Burden 3 Muts/Mb[§]

[§] Refer to appendix for limitation statements related to detection of any copy number alterations, gene rearrangements, BRCA1/2 alterations, LOH, MSI, or TMB results in this section.

Please refer to appendix for Explanation of Clinical Significance Classification and for variants of unknown significance (VUS).

ABOUT THE TEST FoundationOne®CDx is the first FDA-approved broad companion diagnostic for solid tumors.

FoundationOne®CDx (FICDx) is a qualitative next generation sequencing based in vitro diagnostic test that uses targeted high throughput hybridization-based capture technology for detection of substitutions, insertion and deletion alterations (indels), and copy number alterations (CNAs) in 324 genes and select gene rearrangements, as well as genomic signatures including microsatellite instability (MSI) and tumor mutational burden (TMB) using DNA isolated from formalin-fixed, paraffin embedded (FFPE) tumor tissue specimens. The test is intended as a companion diagnostic to identify patients who may benefit from treatment with the targeted therapies listed in Table 1 in accordance with the approved therapeutic product labeling. Additionally, FICDx is intended to provide tumor mutation profiling to be used by qualified health care professionals in accordance with professional guidelines in oncology for patients with solid malignant neoplasms. Genomic findings other than those listed in Table 1 are not prescriptive or conclusive for labeled use of any specific therapeutic product.

The test is also used for detection of genomic loss of heterozygosity (LOH) from formalin-fixed, paraffin-embedded (FFPE) ovarian tumor tissue. Positive homologous recombination deficiency (HRD) status (FICDx HRD defined as tBRCA-positive and/or LOH high) in ovarian cancer patients is associated with improved progression-free survival (PFS) from Rubraca (rucaparib) maintenance therapy in accordance with the Rubraca product label.

The FICDx assay is performed at Foundation Medicine, Inc. sites located in Cambridge, MA and Morrisville, NC.

TABLE 1: COMPANION DIAGNOSTIC INDICATIONS

INDICATIONS	BIOMARKER	THERAPY
Non-small cell lung cancer (NSCLC)	<i>EGFR</i> exon 19 deletions and <i>EGFR</i> exon 21 L858R alterations	Gilotrif® (Afatinib), Iressa® (Gefitinib), Tagrisso® (Osimertinib), or Tarceva® (Erlotinib)
	<i>EGFR</i> exon 20 T790M alterations	Tagrisso® (Osimertinib)
	<i>ALK</i> rearrangements	Alecensa® (Alectinib), Xalkori® (Crizotinib), or Zykadia® (Ceritinib)
	<i>BRAF</i> V600E	Tafinlar® (Dabrafenib) in combination with Mekinist® (Trametinib)
Melanoma	<i>MET</i> single nucleotide variants (SNVs) and indels that lead to <i>MET</i> exon 14 skipping	Tabrecta™ (Capmatinib)
	<i>BRAF</i> V600E and V600K	Tafinlar® (Dabrafenib) or Zelboraf® (Vemurafenib) Mekinist® (Trametinib) or Cotelllic® (Cobimetinib) in combination with Zelboraf® (Vemurafenib)
Breast cancer	<i>ERBB2</i> (HER2) amplification	Herceptin® (Trastuzumab), Kadcyla® (Ado-trastuzumab emtansine), or Perjeta® (Pertuzumab)
	<i>PIK3CA</i> C420R, E542K, E545A, E545D [1635G>T only], E545G, E545K, Q546E, Q546R, H1047L, H1047R, and H1047Y alterations	Piqray® (Alpelisib)
Colorectal cancer	<i>KRAS</i> wild-type (absence of mutations in codons 12 and 13)	Erbix® (Cetuximab)
	<i>KRAS</i> wild-type (absence of mutations in exons 2, 3, and 4) and <i>NRAS</i> wild type (absence of mutations in exons 2, 3, and 4)	Vectibix® (Panitumumab)
Ovarian cancer	<i>BRCA1/2</i> alterations	Lynparza® (Olaparib) or Rubraca® (Rucaparib)
Cholangiocarcinoma	<i>FGFR2</i> fusions and select rearrangements	Pemazyre™ (Pemigatinib)
Prostate cancer	Homologous Recombination Repair (HRR) gene (<i>BRCA1</i> , <i>BRCA2</i> , <i>ATM</i> , <i>BARD1</i> , <i>BRIP1</i> , <i>CDK12</i> , <i>CHEK1</i> , <i>CHEK2</i> , <i>FANCL</i> , <i>PALB2</i> , <i>RAD51B</i> , <i>RAD51C</i> , <i>RAD51D</i> and <i>RAD54L</i>) alterations	Lynparza® (Olaparib)
Solid tumors	TMB ≥ 10 mutations per megabase	Keytruda® (Pembrolizumab)
	<i>NTRK1/2/3</i> fusions	Vitrakvi® (Larotrectinib)

ABOUT THE TEST FoundationOne®CDx is the first FDA-approved broad companion diagnostic for solid tumors.

Electronically signed by Tyler Janovitz, M.D., PhD. | 01 June 2020
 Julia Elvin, M.D., Ph.D., Laboratory Director CLIA: 22D2027531
 Shakti Ramkissoon, M.D., Ph.D., M.M. Sc, Laboratory Director CLIA: 34D2044309
 Foundation Medicine, Inc. | 1-888-988-3639

Sample Preparation: 150 Second St., 1st Floor, Cambridge, MA 02141 • CLIA: 22D2027531
Sample Analysis: 150 Second St., 1st Floor, Cambridge, MA 02141 • CLIA: 22D2027531
Post-Sequencing Analysis: 150 Second St., 1st Floor, Cambridge, MA 02141 • CLIA: 22D2027531

ORDER # ORD-XXXXXX-XX

APPENDIX

About FoundationOne® CDx

INTENDED USE

FoundationOne® CDx (F1CDx) is a qualitative next generation sequencing based *in vitro* diagnostic test that uses targeted high throughput hybridization-based capture technology for detection of substitutions, insertion and deletion alterations (indels), and copy number alterations (CNAs) in 324 genes and select gene rearrangements, as well as genomic signatures including microsatellite instability (MSI) and tumor mutational burden (TMB) using DNA isolated from formalin-fixed, paraffin embedded (FFPE) tumor tissue specimens. The test is intended as a companion diagnostic to identify patients who may benefit from treatment with the targeted therapies listed in Table 1 in accordance with the approved therapeutic product labeling. Additionally, F1CDx is intended to provide tumor mutation profiling to be used by qualified health care professionals in accordance with professional guidelines in oncology for patients with solid malignant neoplasms. Genomic findings other than those listed in Table 1 are not prescriptive or conclusive for labeled use of any specific therapeutic product.

The test is also used for detection of genomic loss of heterozygosity (LOH) from formalin-fixed, paraffin-embedded (FFPE) ovarian tumor tissue. Positive homologous recombination deficiency (HRD) status (F1CDx HRD defined as tBRCA-positive and/or LOH high) in ovarian cancer patients is associated with improved progression-free survival (PFS) from Rubraca (rucaparib) maintenance therapy in accordance with the Rubraca product label.

The F1CDx assay is performed at Foundation Medicine, Inc. sites located in Cambridge, MA and Morrisville, NC

TABLE 1 : COMPANION DIAGNOSTIC INDICATIONS

INDICATION	BIOMARKER	THERAPY
Non-small cell lung cancer (NSCLC)	<i>EGFR</i> exon 19 deletions and <i>EGFR</i> exon 21 L858R alterations	Gilotrif® (Afatinib), Iressa® (Gefitinib), Tagrisso® (Osimertinib), or Tarceva® (Erlotinib)
	<i>EGFR</i> exon 20 T790M alterations	Tagrisso® (Osimertinib)
	<i>ALK</i> rearrangements	Alecensa® (Alectinib), Xalkori® (Crizotinib), or Zykadia® (Ceritinib)
	<i>BRAF</i> V600E	Tafinlar® (Dabrafenib) in combination with Mekinist® (Trametinib)
	<i>MET</i> single nucleotide variants (SNVs) and indels that lead to <i>MET</i> exon 14 skipping	Tabrecta™ (Capmatinib)
Melanoma	<i>BRAF</i> V600E	Tafinlar® (Dabrafenib) or Zelboraf® (Vemurafenib)
	<i>BRAF</i> V600E and V600K	Mekinist® (Trametinib) or Cotellic® (Cobimetinib), in combination with Zelboraf® (Vemurafenib)
Breast cancer	<i>ERBB2</i> (HER2) amplification	Herceptin® (Trastuzumab), Kadcyla® (Ado-trastuzumab emtansine), or Perjeta® (Pertuzumab)
	<i>PIK3CA</i> C420R, E542K, E545A, E545D [1635G>T only], E545G, E545K, Q546E, Q546R, H1047L, H1047R, and H1047Y alterations	Piqray® (Alpelisib)
Colorectal cancer	<i>KRAS</i> wild-type (absence of mutations in codons 12 and 13)	Erbix® (Cetuximab)
	<i>KRAS</i> wild-type (absence of mutations in exons 2, 3, and 4) and <i>NRAS</i> wild type (absence of mutations in exons 2, 3, and 4)	Vectibix® (Panitumumab)
Ovarian cancer	<i>BRCA1/2</i> alterations	Lynparza® (Olaparib) or Rubraca® (Rucaparib)
Cholangiocarcinoma	<i>FGFR2</i> fusions and select rearrangements	Pemazyre™ (Pemigatinib)
Prostate cancer	Homologous Recombination Repair (<i>HRR</i>) gene (<i>BRCA1</i> , <i>BRCA2</i> , <i>ATM</i> , <i>BARD1</i> , <i>BRIPI</i> , <i>CDK12</i> , <i>CHEK1</i> , <i>CHEK2</i> , <i>FANCL</i> , <i>PALB2</i> , <i>RAD51B</i> , <i>RAD51C</i> , <i>RAD51D</i> and <i>RAD54L</i>) alterations	Lynparza® (Olaparib)
Solid tumors	TMB ≥ 10 mutations per megabase	Keytruda® (Pembrolizumab)
	<i>NTRK1/2/3</i> fusions	Vitrakvi® (Larotrectinib)

The median exon coverage for this sample is 827x

ORDER # ORD-XXXXXX-XX

APPENDIX About FoundationOne®CDx

TEST PRINCIPLE

FoundationOne®CDx (F1CDx) is performed exclusively as a laboratory service using DNA extracted from formalin-fixed, paraffin-embedded (FFPE) tumor samples. The assay employs a single DNA extraction method from routine FFPE biopsy or surgical resection specimens, 50-1000 ng of which will undergo whole-genome shotgun library construction and hybridization-based capture of all coding exons from 309 cancer-related genes, one promoter region, one non-coding (ncRNA), and select intronic regions from 34 commonly rearranged genes, 21 of which also include the coding exons (refer to Table 2 and Table 3 for complete list of genes included in F1CDx). In total, the assay detects alterations in a total of 324 genes. Using the Illumina® HiSeq 4000 platform, hybrid capture-selected libraries are sequenced to high uniform depth (targeting >500X median coverage with >99% of exons at coverage >100X). Sequence data is then processed using a customized analysis pipeline designed to detect all classes of genomic alterations, including base substitutions, indels, copy number alterations (amplifications and homozygous gene deletions), and selected genomic rearrangements (e.g., gene fusions). Additionally, genomic signatures including microsatellite instability (MSI), tumor mutational burden (TMB), and positive homologous recombination deficiency (HRD) status (tBRCA-positive and/or LOH high) are reported.

PERFORMANCE CHARACTERISTICS

Please refer to product label:
foundationmedicine.com/f1cdx

WARNINGS AND PRECAUTIONS

- Alterations reported may include somatic (not inherited) or germline (inherited) alterations; however, the test does not distinguish between germline and somatic alterations. The test does not provide information about susceptibility.
- Biopsy may pose a risk to the patient when archival tissue is not available for use with the assay. The patient's physician should determine whether the patient is a candidate for biopsy.
- Reflex testing to an alternative FDA approved companion diagnostic should be performed for patients who have an *ERBB2* amplification result detected with copy number equal to 4 (baseline ploidy of tumor +2) for confirmatory testing. While this result is considered negative by FoundationOne®CDx (F1CDx), in a clinical concordance study with an FDA approved FISH test, 70% (7 out of 10 samples) were positive, and 30% (3 out of 10 samples) were negative by the FISH test with an average ratio of 2.3. The frequency of *ERBB2* copy number 4 in breast cancer is estimated to be approximately 2%.

Multiple references listed in <https://www.mycancergenome.org/content/disease/breast-cancer/ERBB2/238/>) report the frequency of HER2 overexpression as 20% in breast cancer. Based on the F1CDx HER2 CDx concordance study, approximately 10% of HER2 amplified samples had copy number 4. Thus, total frequency is conservatively estimated to be approximately 2%.

LIMITATIONS

- For *in vitro* diagnostic use.
- For prescription use only. This test must be ordered by a qualified medical professional in accordance with clinical laboratory regulations.
- A negative result does not rule out the presence of a mutation below the limits of detection of the assay.
- Samples with <25% tumor may have decreased sensitivity for the detection of CNAs including *ERBB2*.
- Clinical performance of Tagrisso® (osimertinib) in patients with an *EGFR* exon 20 T790M mutation detected with an allele fraction <5% is ongoing and has not been established.
- Concordance with other validated methods for CNA (with the exception of *ERBB2*) and gene rearrangement (with the exception of *ALK*) detection has not been demonstrated and will be provided in the post-market setting. Confirmatory testing using a clinically validated assay should be performed for all CNAs and rearrangements not associated with CDx claims noted in Table 1 of the Intended Use, but used for clinical decision making.
- The MSI-H/MSS designation by FMI FoundationOne®CDx (F1CDx) test is based on genome wide analysis of 95 microsatellite loci and not based on the 5 or 7 MSI loci described in current clinical practice guidelines. Refer https://www.accessdata.fda.gov/cdrh_docs/pdf17/P170019B.pdf for additional details on methodology. The threshold for MSI-H/MSS was determined by analytical concordance to comparator assays (IHC and PCR) using uterine, cecum and colorectal cancer FFPE tissue. Patients with microsatellite status of "Cannot Be Determined" should be retested with an orthogonal (alternative) method. The clinical validity of the qualitative MSI designation has not been established.
- TMB by F1CDx is determined by counting all synonymous and non-synonymous variants present at 5% allele frequency or greater (after filtering) and the total number is reported as mutations per megabase (mut/Mb) unit. Observed TMB is dependent on characteristics of the specific tumor focus tested for a patient (e.g., primary vs. metastatic, tumor content) and the testing platform used for the detection; therefore, observed TMB results may vary

- between different specimens for the same patient and between detection methodologies employed on the same sample. The TMB calculation may differ from TMB calculations used by other assays depending on variables such as the amount of genome interrogated, percentage of tumor, assay limit of detection (LoD), filtering of alterations included in the score, and the read depth and other bioinformatic test specifications. Refer to the SSED for a detailed description of these variables in FMI's TMB calculation https://www.accessdata.fda.gov/cdrh_docs/pdf17/P170019B.pdf. The clinical validity of TMB defined by this panel has been established for TMB as a qualitative output for a cut-off of 10 mutations per megabase but has not been established for TMB as a quantitative score.
- Decisions on patient care and treatment must be based on the independent medical judgment of the treating physician, taking into consideration all applicable information concerning the patient's condition, such as patient and family history, physical examinations, information from other diagnostic tests, and patient preferences, in accordance with the standard of care in a given community.
 - The test is intended to be performed on specific serial number-controlled instruments by Foundation Medicine, Inc.
 - Alterations in polyT homopolymer runs may not be reliably detected in *BRCA1/2*.
 - Certain large rearrangements in *BRCA1/2* including large scale genomic deletions (affecting at least one whole exon), insertions or other deleterious genomic rearrangements including inversions or transversion events, may not be detected in an estimated 5% of ovarian cancer patients with *BRCA1/2* mutations by F1CDx.
 - Certain potentially deleterious missense or small in-frame deletions in *BRCA1/2* may not be reported under the "CDx associated findings" but may be reported in the "Other alterations and biomarkers identified" section in the patient report.
 - Alterations at allele frequencies below the established limit of detection may not be detected consistently.
 - Detection of LOH has been verified only for ovarian cancer patients.
 - Performance of the LOH classification has not been established for samples below 35% tumor content and with LOH scores near the cutoff of 16.
 - There may be potential interference of ethanol with LOH detection. The interfering effects of xylene, hemoglobin, and triglycerides on the LOH score have not been demonstrated.
 - While the overall positive percent agreement

ORDER # ORD-XXXXXX-XX

APPENDIX

About FoundationOne® CDx

between trial enrollment assays and F1CDx was 84% (37/44), thirty percent (30%) (6/20) of patients enrolled in the VITRAKVI clinical studies using RNA-based NGS detection were negative for *NTRK* fusions by F1CDx. Four of the six patients (4/6 or 60%) that were negative for *NTRK* fusions by F1CDx had a response to larotrectinib. Therefore, F1CDx may miss a subset of patients with solid tumors with *NTRK1/2/3* fusions who may derive benefit from VITRAKVI.

19. *NTRK2* fusions per the F1CDx CDx biomarker rules for *NTRK1/2/3* fusions were not well-represented in analytical validation studies.

PDF Service Version o.o.o

APPENDIX
Genes assayed in FoundationOne®CDx

ORDERED TEST #

FoundationOne CDx is designed to include genes known to be somatically altered in human solid tumors that are validated targets for therapy, either approved or in clinical trials, and/or that are unambiguous drivers of oncogenesis based on current knowledge. The current assay interrogates 324 genes as well as introns of 36 genes involved in rearrangements. The assay will be updated periodically to reflect new knowledge about cancer biology.

DNA GENE LIST: ENTIRE CODING SEQUENCE FOR THE DETECTION OF BASE SUBSTITUTIONS, INSERTION/DELETIONS, AND COPY NUMBER ALTERATIONS

ABL1	ACVR1B	AKT1	AKT2	AKT3	ALK	ALOX12B	AMER1 (FAM123B)	APC
AR	ARAF	ARFRP1	ARID1A	ASXL1	ATM	ATR	ATRX	AURKA
AURKB	AXIN1	AXL	BAP1	BARD1	BCL2	BCL2L1	BCL2L2	BCL6
BCOR	BCORL1	BRAF	BRCA1	BRCA2	BRD4	BRIP1	BTG1	BTG2
BTK	C11orf30 (EMSY)	C17orf39 (GID4)	CALR	CARD11	CASP8	CBFB	CBL	CCND1
CCND2	CCND3	CCNE1	CD22	CD274 (PD-L1)	CD70	CD79A	CD79B	CDC73
CDH1	CDK12	CDK4	CDK6	CDK8	CDKN1A	CDKN1B	CDKN2A	CDKN2B
CDKN2C	CEBPA	CHEK1	CHEK2	CIC	CREBBP	CRKL	CSF1R	CSF3R
CTCF	CTNNA1	CTNNB1	CUL3	CUL4A	CXCR4	CYP17A1	DAXX	DDR1
DDR2	DIS3	DNMT3A	DOT1L	EED	EGFR	EP300	EPHA3	EPHB1
EPHB4	ERBB2	ERBB3	ERBB4	ERCC4	ERG	ERRF1	ESR1	EZH2
FAM46C	FANCA	FANCC	FANCG	FANCL	FAS	FBXW7	FGF10	FGF12
FGF14	FGF19	FGF23	FGF3	FGF4	FGF6	FGFR1	FGFR2	FGFR3
FGFR4	FH	FLCN	FLT1	FLT3	FOXL2	FUBP1	GABRA6	GATA3
GATA4	GATA6	GNA11	GNA13	GNAQ	GNAS	GRM3	GSK3B	H3F3A
HDAC1	HGF	HNF1A	HRAS	HSD3B1	ID3	IDH1	IDH2	IGF1R
IKBKE	IKZF1	INPP4B	IRF2	IRF4	IRS2	JAK1	JAK2	JAK3
JUN	KDMSA	KDMS5C	KDM6A	KDR	KEAP1	KEL	KIT	KLHL6
KMT2A (MLL)	KMT2D (MLL2)	KRAS	LTK	LYN	MAF	MAP2K1 (MEK1)	MAP2K2 (MEK2)	MAP2K4
MAP3K1	MAP3K13	MAPK1	MCL1	MDM2	MDM4	MED12	MEF2B	MEN1
MERTK	MET	MITF	MKNK1	MLH1	MPL	MRE11A	MSH2	MSH3
MSH6	MST1R	MTAP	MTOR	MUTYH	MYC	MYCL (MYCL1)	MYCN	MYD88
NBN	NF1	NF2	NFE2L2	NFKBIA	NKX2-1	NOTCH1	NOTCH2	NOTCH3
NPM1	NRAS	NSD3 (WHSC1L1)	NT5C2	NTRK1	NTRK2	NTRK3	P2RY8	PALB2
PARK2	PARP1	PARP2	PARP3	PAX5	PBRM1	PDCD1 (PD-1)	PDCD1LG2 (PD-L2)	PDGFRA
PDGFRB	PDK1	PIK3C2B	PIK3C2G	PIK3CA	PIK3CB	PIK3R1	PIM1	PMS2
POLD1	POLE	PPARG	PPP2R1A	PPP2R2A	PRDM1	PRKARIA	PRKCI	PTCH1
PTEN	PTPN11	PTPRO	QKI	RAC1	RAD21	RAD51	RAD51B	RAD51C
RAD51D	RAD52	RAD54L	RAF1	RARA	RB1	RBM10	REL	RET
RICTOR	RNF43	ROS1	RPTOR	SDHA	SDHB	SDHC	SDHD	SETD2
SF3B1	SGK1	SMAD2	SMAD4	SMARCA4	SMARCB1	SMO	SNCAIP	SOCS1
SOX2	SOX9	SPEX1	SPOP	SRC	STAG2	STAT3	STK11	SUFU
SYK	TBX3	TEK	TET2	TGFBR2	TIPARP	TNFAIP3	TNFRSF14	TP53
TSC1	TSC2	TYRO3	U2AF1	VEGFA	VHL	WHSC1	WT1	XPO1
XRCC2	ZNF217	ZNF703						

DNA GENE LIST: FOR THE DETECTION OF SELECT REARRANGEMENTS

ALK	BCL2	BCR	BRAF	BRCA1	BRCA2	CD74	EGFR	ETV4
ETV5	ETV6	EWSR1	EZR	FGFR1	FGFR2	FGFR3	KIT	KMT2A (MLL)
MSH2	MYB	MYC	NOTCH2	NTRK1	NTRK2	NUTM1	PDGFRA	RAF1
RARA	RET	ROS1	RSPO2	SDC4	SLC34A2	TERC*	TERT**	TMPPRSS2

*TERC is an NCRNA

**Promoter region of TERT is interrogated

ADDITIONAL ASSAYS: FOR THE DETECTION OF SELECT CANCER BIOMARKERS

Loss of Heterozygosity (LOH) score
 Microsatellite (MS) status
 Tumor Mutational Burden (TMB)

PATIENT

DISEASE Unknown primary malignant neoplasm
NAME Not Given
DATE OF BIRTH Not Given
SEX Not Given
MEDICAL RECORD # Not Given

PHYSICIAN

ORDERING PHYSICIAN Not Given
MEDICAL FACILITY Not Given
ADDITIONAL RECIPIENT Not Given
MEDICAL FACILITY ID Not Given
PATHOLOGIST Not Given

SPECIMEN

SPECIMEN SITE Not Given
SPECIMEN ID Not Given
SPECIMEN TYPE Not Given
DATE OF COLLECTION Not Given
SPECIMEN RECEIVED Not Given

NO REPORTABLE ALTERATIONS WITH COMPANION DIAGNOSTIC (CDx) CLAIMS

See professional services section for additional information

For Microsatellite Instability (MSI) results, confirmatory testing using a validated orthogonal method should be performed.

OTHER ALTERATIONS & BIOMARKERS IDENTIFIED

Results reported in this section are not prescriptive or conclusive for labeled use of any specific therapeutic product.
See professional services section for additional information.

Microsatellite status MS-Stable [§]	(T4; P18) [§]
Tumor Mutational Burden 3 Muts/Mb [§]	TMPRSS2 TMPRSS2(NM_005656)-ERG(NM_004449) fusion
AR amplification [§]	(T1; E4) [§]
NTRK3 NTRK3(NM_002530) rearrangement intron 14 [§]	TP53 R273C
PDGFRA THAP6(NM_144721)-PDGFRA(NM_006206) fusion	

[§] Refer to appendix for limitation statements related to detection of any copy number alterations, gene rearrangements, BRCA1/2 alterations, LOH, MSI, or TMB results in this section.

Please refer to appendix for Explanation of Clinical Significance Classification and for variants of unknown significance (VUS).

ABOUT THE TEST FoundationOne®CDx is the first FDA-approved broad companion diagnostic for solid tumors.

FoundationOne®CDx (FICDx) is a qualitative next generation sequencing based in vitro diagnostic test that uses targeted high throughput hybridization-based capture technology for detection of substitutions, insertion and deletion alterations (indels), and copy number alterations (CNAs) in 324 genes and select gene rearrangements, as well as genomic signatures including microsatellite instability (MSI) and tumor mutational burden (TMB) using DNA isolated from formalin-fixed, paraffin embedded (FFPE) tumor tissue specimens. The test is intended as a companion diagnostic to identify patients who may benefit from treatment with the targeted therapies listed in Table 1 in accordance with the approved therapeutic product labeling. Additionally, FICDx is intended to provide tumor mutation profiling to be used by qualified health care professionals in accordance with professional guidelines in oncology for patients with solid malignant neoplasms. Genomic findings other than those listed in Table 1 are not prescriptive or conclusive for labeled use of any specific therapeutic product.

The test is also used for detection of genomic loss of heterozygosity (LOH) from formalin-fixed, paraffin-embedded (FFPE) ovarian tumor tissue. Positive homologous recombination deficiency (HRD) status (FICDx HRD defined as tBRCA-positive and/or LOH high) in ovarian cancer patients is associated with improved progression-free survival (PFS) from Rubraca (rucaparib) maintenance therapy in accordance with the Rubraca product label.

The FICDx assay is performed at Foundation Medicine, Inc. sites located in Cambridge, MA and Morrisville, NC.

TABLE 1: COMPANION DIAGNOSTIC INDICATIONS

INDICATIONS	BIOMARKER	THERAPY
Non-small cell lung cancer (NSCLC)	<i>EGFR</i> exon 19 deletions and <i>EGFR</i> exon 21 L858R alterations	Gilotrif® (Afatinib), Iressa® (Gefitinib), Tagrisso® (Osimertinib), or Tarceva® (Erlotinib)
	<i>EGFR</i> exon 20 T790M alterations	Tagrisso® (Osimertinib)
	<i>ALK</i> rearrangements	Alecensa® (Alectinib), Xalkori® (Crizotinib), or Zykadia® (Ceritinib)
	<i>BRAF</i> V600E	Tafinlar® (Dabrafenib) in combination with Mekinist® (Trametinib)
Melanoma	<i>MET</i> single nucleotide variants (SNVs) and indels that lead to <i>MET</i> exon 14 skipping	Tabrecta™ (Capmatinib)
	<i>BRAF</i> V600E	Tafinlar® (Dabrafenib) or Zelboraf® (Vemurafenib)
Breast cancer	<i>BRAF</i> V600E and V600K	Mekinist® (Trametinib) or Cotelllic® (Cobimetinib) in combination with Zelboraf® (Vemurafenib)
	<i>ERBB2</i> (HER2) amplification	Herceptin® (Trastuzumab), Kadcyla® (Ado-trastuzumab emtansine), or Perjeta® (Pertuzumab)
Colorectal cancer	<i>PIK3CA</i> C420R, E542K, E545A, E545D [1635G>T only], E545G, E545K, Q546E, Q546R, H1047L, H1047R, and H1047Y alterations	Piqray® (Alpelisib)
	<i>KRAS</i> wild-type (absence of mutations in codons 12 and 13)	Erbix® (Cetuximab)
Ovarian cancer	<i>KRAS</i> wild-type (absence of mutations in exons 2, 3, and 4) and <i>NRAS</i> wild type (absence of mutations in exons 2, 3, and 4)	Vectibix® (Panitumumab)
	<i>BRCA1/2</i> alterations	Lynparza® (Olaparib) or Rubraca® (Rucaparib)
Cholangiocarcinoma	<i>FGFR2</i> fusions and select rearrangements	Pemazyre™ (Pemigatinib)
Prostate cancer	Homologous Recombination Repair (HRR) gene (<i>BRCA1</i> , <i>BRCA2</i> , <i>ATM</i> , <i>BARD1</i> , <i>BRIP1</i> , <i>CDK12</i> , <i>CHEK1</i> , <i>CHEK2</i> , <i>FANCL</i> , <i>PALB2</i> , <i>RAD51B</i> , <i>RAD51C</i> , <i>RAD51D</i> and <i>RAD54L</i>) alterations	Lynparza® (Olaparib)
Solid tumors	TMB ≥ 10 mutations per megabase	Keytruda® (Pembrolizumab)
	<i>NTRK1/2/3</i> fusions	Vitakvi® (Larotrectinib)

ABOUT THE TEST FoundationOne®CDx is the first FDA-approved broad companion diagnostic for solid tumors.

Electronically signed by Tyler Janovitz, M.D., PhD. | 01 June 2020
 Julia Elvin, M.D., Ph.D., Laboratory Director CLIA: 22D2027531
 Shakti Ramkissoon, M.D., Ph.D., M.M. Sc, Laboratory Director CLIA: 34D2044309
 Foundation Medicine, Inc. | 1-888-988-3639

Sample Preparation: 150 Second St., 1st Floor, Cambridge, MA 02141 • CLIA: 22D2027531
Sample Analysis: 150 Second St., 1st Floor, Cambridge, MA 02141 • CLIA: 22D2027531
Post-Sequencing Analysis: 150 Second St., 1st Floor, Cambridge, MA 02141 • CLIA: 22D2027531

ORDER # ORD-XXXXXX-XX

APPENDIX

About FoundationOne® CDx

INTENDED USE

FoundationOne® CDx (F1CDx) is a qualitative next generation sequencing based *in vitro* diagnostic test that uses targeted high throughput hybridization-based capture technology for detection of substitutions, insertion and deletion alterations (indels), and copy number alterations (CNAs) in 324 genes and select gene rearrangements, as well as genomic signatures including microsatellite instability (MSI) and tumor mutational burden (TMB) using DNA isolated from formalin-fixed, paraffin embedded (FFPE) tumor tissue specimens. The test is intended as a companion diagnostic to identify patients who may benefit from treatment with the targeted therapies listed in Table 1 in accordance with the approved therapeutic product labeling. Additionally, F1CDx is intended to provide tumor mutation profiling to be used by qualified health care professionals in accordance with professional guidelines in oncology for patients with solid malignant neoplasms. Genomic findings other than those listed in Table 1 are not prescriptive or conclusive for labeled use of any specific therapeutic product.

The test is also used for detection of genomic loss of heterozygosity (LOH) from formalin-fixed, paraffin-embedded (FFPE) ovarian tumor tissue. Positive homologous recombination deficiency (HRD) status (F1CDx HRD defined as tBRCA-positive and/or LOH high) in ovarian cancer patients is associated with improved progression-free survival (PFS) from Rubraca (rucaparib) maintenance therapy in accordance with the Rubraca product label.

The F1CDx assay is performed at Foundation Medicine, Inc. sites located in Cambridge, MA and Morrisville, NC

TABLE 1 : COMPANION DIAGNOSTIC INDICATIONS

INDICATION	BIOMARKER	THERAPY
Non-small cell lung cancer (NSCLC)	<i>EGFR</i> exon 19 deletions and <i>EGFR</i> exon 21 L858R alterations	Gilotrif® (Afatinib), Iressa® (Gefitinib), Tagrisso® (Osimertinib), or Tarceva® (Erlotinib)
	<i>EGFR</i> exon 20 T790M alterations	Tagrisso® (Osimertinib)
	<i>ALK</i> rearrangements	Alecensa® (Alectinib), Xalkori® (Crizotinib), or Zykadia® (Ceritinib)
	<i>BRAF</i> V600E	Tafinlar® (Dabrafenib) in combination with Mekinist® (Trametinib)
	<i>MET</i> single nucleotide variants (SNVs) and indels that lead to <i>MET</i> exon 14 skipping	Tabrecta™ (Capmatinib)
Melanoma	<i>BRAF</i> V600E	Tafinlar® (Dabrafenib) or Zelboraf® (Vemurafenib)
	<i>BRAF</i> V600E and V600K	Mekinist® (Trametinib) or Cotellic® (Cobimetinib), in combination with Zelboraf® (Vemurafenib)
Breast cancer	<i>ERBB2</i> (HER2) amplification	Herceptin® (Trastuzumab), Kadcyla® (Ado-trastuzumab emtansine), or Perjeta® (Pertuzumab)
	<i>PIK3CA</i> C420R, E542K, E545A, E545D [1635G>T only], E545G, E545K, Q546E, Q546R, H1047L, H1047R, and H1047Y alterations	Piqray® (Alpelisib)
Colorectal cancer	<i>KRAS</i> wild-type (absence of mutations in codons 12 and 13)	Erbix® (Cetuximab)
	<i>KRAS</i> wild-type (absence of mutations in exons 2, 3, and 4) and <i>NRAS</i> wild type (absence of mutations in exons 2, 3, and 4)	Vectibix® (Panitumumab)
Ovarian cancer	<i>BRCA1/2</i> alterations	Lynparza® (Olaparib) or Rubraca® (Rucaparib)
Cholangiocarcinoma	<i>FGFR2</i> fusions and select rearrangements	Pemazyre™ (Pemigatinib)
Prostate cancer	Homologous Recombination Repair (<i>HRR</i>) gene (<i>BRCA1</i> , <i>BRCA2</i> , <i>ATM</i> , <i>BARD1</i> , <i>BRIPI</i> , <i>CDK12</i> , <i>CHEK1</i> , <i>CHEK2</i> , <i>FANCL</i> , <i>PALB2</i> , <i>RAD51B</i> , <i>RAD51C</i> , <i>RAD51D</i> and <i>RAD54L</i>) alterations	Lynparza® (Olaparib)
Solid tumors	<i>TMB</i> ≥ 10 mutations per megabase	Keytruda® (Pembrolizumab)
	<i>NTRK1/2/3</i> fusions	Vitrakvi® (Larotrectinib)

The median exon coverage for this sample is 827x

ORDER # ORD-XXXXXX-XX

APPENDIX About FoundationOne®CDx

TEST PRINCIPLE

FoundationOne®CDx (F1CDx) is performed exclusively as a laboratory service using DNA extracted from formalin-fixed, paraffin-embedded (FFPE) tumor samples. The assay employs a single DNA extraction method from routine FFPE biopsy or surgical resection specimens, 50-1000 ng of which will undergo whole-genome shotgun library construction and hybridization-based capture of all coding exons from 309 cancer-related genes, one promoter region, one non-coding (ncRNA), and select intronic regions from 34 commonly rearranged genes, 21 of which also include the coding exons (refer to Table 2 and Table 3 for complete list of genes included in F1CDx). In total, the assay detects alterations in a total of 324 genes. Using the Illumina® HiSeq 4000 platform, hybrid capture-selected libraries are sequenced to high uniform depth (targeting >500X median coverage with >99% of exons at coverage >100X). Sequence data is then processed using a customized analysis pipeline designed to detect all classes of genomic alterations, including base substitutions, indels, copy number alterations (amplifications and homozygous gene deletions), and selected genomic rearrangements (e.g., gene fusions). Additionally, genomic signatures including microsatellite instability (MSI), tumor mutational burden (TMB), and positive homologous recombination deficiency (HRD) status (tBRCA-positive and/or LOH high) are reported.

PERFORMANCE CHARACTERISTICS

Please refer to product label:
foundationmedicine.com/f1cdx

WARNINGS AND PRECAUTIONS

1. Alterations reported may include somatic (not inherited) or germline (inherited) alterations; however, the test does not distinguish between germline and somatic alterations. The test does not provide information about susceptibility.
2. Biopsy may pose a risk to the patient when archival tissue is not available for use with the assay. The patient's physician should determine whether the patient is a candidate for biopsy.
3. Reflex testing to an alternative FDA approved companion diagnostic should be performed for patients who have an *ERBB2* amplification result detected with copy number equal to 4 (baseline ploidy of tumor +2) for confirmatory testing. While this result is considered negative by FoundationOne®CDx (F1CDx), in a clinical concordance study with an FDA approved FISH test, 70% (7 out of 10 samples) were positive, and 30% (3 out of 10 samples) were negative by the FISH test with an average ratio of 2.3. The frequency of *ERBB2* copy number 4 in breast cancer is estimated to be approximately 2%.

Multiple references listed in <https://www.mycancergenome.org/content/disease/breast-cancer/ERBB2/238/>) report the frequency of HER2 overexpression as 20% in breast cancer. Based on the F1CDx HER2 CDx concordance study, approximately 10% of HER2 amplified samples had copy number 4. Thus, total frequency is conservatively estimated to be approximately 2%.

LIMITATIONS

1. For *in vitro* diagnostic use.
2. For prescription use only. This test must be ordered by a qualified medical professional in accordance with clinical laboratory regulations.
3. A negative result does not rule out the presence of a mutation below the limits of detection of the assay.
4. Samples with <25% tumor may have decreased sensitivity for the detection of CNAs including *ERBB2*.
5. Clinical performance of Tagrisso® (osimertinib) in patients with an *EGFR* exon 20 T790M mutation detected with an allele fraction <5% is ongoing and has not been established.
6. Concordance with other validated methods for CNA (with the exception of *ERBB2*) and gene rearrangement (with the exception of *ALK*) detection has not been demonstrated and will be provided in the post-market setting. Confirmatory testing using a clinically validated assay should be performed for all CNAs and rearrangements not associated with CDx claims noted in Table 1 of the Intended Use, but used for clinical decision making.
7. The MSI-H/MSS designation by FMI FoundationOne®CDx (F1CDx) test is based on genome wide analysis of 95 microsatellite loci and not based on the 5 or 7 MSI loci described in current clinical practice guidelines. Refer https://www.accessdata.fda.gov/cdrh_docs/pdf17/P170019B.pdf for additional details on methodology. The threshold for MSI-H/MSS was determined by analytical concordance to comparator assays (IHC and PCR) using uterine, cecum and colorectal cancer FFPE tissue. Patients with microsatellite status of "Cannot Be Determined" should be retested with an orthogonal (alternative) method. The clinical validity of the qualitative MSI designation has not been established.
8. TMB by F1CDx is determined by counting all synonymous and non-synonymous variants present at 5% allele frequency or greater (after filtering) and the total number is reported as mutations per megabase (mut/Mb) unit. Observed TMB is dependent on characteristics of the specific tumor focus tested for a patient (e.g., primary vs. metastatic, tumor content) and the testing platform used for the detection; therefore, observed TMB results may vary

- between different specimens for the same patient and between detection methodologies employed on the same sample. The TMB calculation may differ from TMB calculations used by other assays depending on variables such as the amount of genome interrogated, percentage of tumor, assay limit of detection (LoD), filtering of alterations included in the score, and the read depth and other bioinformatic test specifications. Refer to the SSED for a detailed description of these variables in FMI's TMB calculation https://www.accessdata.fda.gov/cdrh_docs/pdf17/P170019B.pdf. The clinical validity of TMB defined by this panel has been established for TMB as a qualitative output for a cut-off of 10 mutations per megabase but has not been established for TMB as a quantitative score.
9. Decisions on patient care and treatment must be based on the independent medical judgment of the treating physician, taking into consideration all applicable information concerning the patient's condition, such as patient and family history, physical examinations, information from other diagnostic tests, and patient preferences, in accordance with the standard of care in a given community.
 10. The test is intended to be performed on specific serial number-controlled instruments by Foundation Medicine, Inc.
 11. Alterations in polyT homopolymer runs may not be reliably detected in *BRCA1/2*.
 12. Certain large rearrangements in *BRCA1/2* including large scale genomic deletions (affecting at least one whole exon), insertions or other deleterious genomic rearrangements including inversions or transversion events, may not be detected in an estimated 5% of ovarian cancer patients with *BRCA1/2* mutations by F1CDx.
 13. Certain potentially deleterious missense or small in-frame deletions in *BRCA1/2* may not be reported under the "CDx associated findings" but may be reported in the "Other alterations and biomarkers identified" section in the patient report.
 14. Alterations at allele frequencies below the established limit of detection may not be detected consistently.
 15. Detection of LOH has been verified only for ovarian cancer patients.
 16. Performance of the LOH classification has not been established for samples below 35% tumor content and with LOH scores near the cutoff of 16.
 17. There may be potential interference of ethanol with LOH detection. The interfering effects of xylene, hemoglobin, and triglycerides on the LOH score have not been demonstrated.
 18. While the overall positive percent agreement

ORDER # ORD-XXXXXX-XX

APPENDIX

About FoundationOne® CDx

between trial enrollment assays and F1CDx was 84% (37/44), thirty percent (30%) (6/20) of patients enrolled in the VITRAKVI clinical studies using RNA-based NGS detection were negative for *NTRK* fusions by F1CDx. Four of the six patients (4/6 or 60%) that were negative for *NTRK* fusions by F1CDx had a response to larotrectinib. Therefore, F1CDx may miss a subset of patients with solid tumors with *NTRK1/2/3* fusions who may derive benefit from VITRAKVI.

19. *NTRK2* fusions per the F1CDx CDx biomarker rules for *NTRK1/2/3* fusions were not well-represented in analytical validation studies.

PDF Service Version o.o.o

APPENDIX

Genes assayed in FoundationOne®CDx

ORDERED TEST #

FoundationOne CDx is designed to include genes known to be somatically altered in human solid tumors that are validated targets for therapy, either approved or in clinical trials, and/or that are unambiguous drivers of oncogenesis based on current knowledge. The current assay interrogates 324 genes as well as introns of 36 genes involved in rearrangements. The assay will be updated periodically to reflect new knowledge about cancer biology.

DNA GENE LIST: ENTIRE CODING SEQUENCE FOR THE DETECTION OF BASE SUBSTITUTIONS, INSERTION/DELETIONS, AND COPY NUMBER ALTERATIONS

ABL1	ACVR1B	AKT1	AKT2	AKT3	ALK	ALOX12B	AMER1 (FAM123B)	APC
AR	ARAF	ARFRP1	ARID1A	ASXL1	ATM	ATR	ATRX	AURKA
AURKB	AXIN1	AXL	BAP1	BARD1	BCL2	BCL2L1	BCL2L2	BCL6
BCOR	BCORL1	BRAF	BRCA1	BRCA2	BRD4	BRIP1	BTG1	BTG2
BTK	C11orf30 (EMSY)	C17orf39 (GID4)	CALR	CARD11	CASP8	CBFB	CBL	CCND1
CCND2	CCND3	CCNE1	CD22	CD274 (PD-L1)	CD70	CD79A	CD79B	CDC73
CDH1	CDK12	CDK4	CDK6	CDK8	CDKN1A	CDKN1B	CDKN2A	CDKN2B
CDKN2C	CEBPA	CHEK1	CHEK2	CIC	CREBBP	CRKL	CSF1R	CSF3R
CTCF	CTNNA1	CTNNB1	CUL3	CUL4A	CXCR4	CYP17A1	DAXX	DDR1
DDR2	DIS3	DNMT3A	DOT1L	EED	EGFR	EP300	EPHA3	EPHB1
EPHB4	ERBB2	ERBB3	ERBB4	ERCC4	ERG	ERRF1	ESR1	EZH2
FAM46C	FANCA	FANCC	FANCG	FANCL	FAS	FBXW7	FGF10	FGF12
FGF14	FGF19	FGF23	FGF3	FGF4	FGF6	FGFR1	FGFR2	FGFR3
FGFR4	FH	FLCN	FLT1	FLT3	FOXL2	FUBP1	GABRA6	GATA3
GATA4	GATA6	GNA11	GNA13	GNAQ	GNAS	GRM3	GSK3B	H3F3A
HDAC1	HGF	HNF1A	HRAS	HSD3B1	ID3	IDH1	IDH2	IGF1R
IKBKE	IKZF1	INPP4B	IRF2	IRF4	IRS2	JAK1	JAK2	JAK3
JUN	KDMSA	KDMS5C	KDM6A	KDR	KEAP1	KEL	KIT	KLHL6
KMT2A (MLL)	KMT2D (MLL2)	KRAS	LTK	LYN	MAF	MAP2K1 (MEK1)	MAP2K2 (MEK2)	MAP2K4
MAP3K1	MAP3K13	MAPK1	MCL1	MDM2	MDM4	MED12	MEF2B	MEN1
MERTK	MET	MITF	MKNK1	MLH1	MPL	MRE11A	MSH2	MSH3
MSH6	MST1R	MTAP	MTOR	MUTYH	MYC	MYCL (MYCL1)	MYCN	MYD88
NBN	NF1	NF2	NFE2L2	NFKBIA	NKX2-1	NOTCH1	NOTCH2	NOTCH3
NPM1	NRAS	NSD3 (WHSC1L1)	NT5C2	NTRK1	NTRK2	NTRK3	P2RY8	PALB2
PARK2	PARP1	PARP2	PARP3	PAX5	PBRM1	PDCD1 (PD-1)	PDCD1LG2 (PD-L2)	PDGFRA
PDGFRB	PDK1	PIK3C2B	PIK3C2G	PIK3CA	PIK3CB	PIK3R1	PIM1	PMS2
POLD1	POLE	PPARG	PPP2R1A	PPP2R2A	PRDM1	PRKARIA	PRKCI	PTCH1
PTEN	PTPN11	PTPRO	QKI	RAC1	RAD21	RAD51	RAD51B	RAD51C
RAD51D	RAD52	RAD54L	RAF1	RARA	RB1	RBM10	REL	RET
RICTOR	RNF43	ROS1	RPTOR	SDHA	SDHB	SDHC	SDHD	SETD2
SF3B1	SGK1	SMAD2	SMAD4	SMARCA4	SMARCB1	SMO	SNCAIP	SOCS1
SOX2	SOX9	SPEX1	SPOP	SRC	STAG2	STAT3	STK11	SUFU
SYK	TBX3	TEK	TET2	TGFBR2	TIPARP	TNFAIP3	TNFRSF14	TP53
TSC1	TSC2	TYRO3	U2AF1	VEGFA	VHL	WHSC1	WT1	XPO1
XRCC2	ZNF217	ZNF703						

DNA GENE LIST: FOR THE DETECTION OF SELECT REARRANGEMENTS

ALK	BCL2	BCR	BRAF	BRCA1	BRCA2	CD74	EGFR	ETV4
ETV5	ETV6	EWSR1	EZR	FGFR1	FGFR2	FGFR3	KIT	KMT2A (MLL)
MSH2	MYB	MYC	NOTCH2	NTRK1	NTRK2	NUTM1	PDGFRA	RAF1
RARA	RET	ROS1	RSPO2	SDC4	SLC34A2	TERC*	TERT**	TMPPSS2

*TERC is an NCRNA

**Promoter region of TERT is interrogated

ADDITIONAL ASSAYS: FOR THE DETECTION OF SELECT CANCER BIOMARKERS

- Loss of Heterozygosity (LOH) score
- Microsatellite (MS) status
- Tumor Mutational Burden (TMB)